

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059736.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157207BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.832	408	416	423	rBV	501150	791825	22.66%	6.921%
2	7.459	684	693	704	rVB	533295	927312	26.53%	8.105%
3	8.340	834	843	849	rVB2	97405	174050	4.98%	1.521%
4	9.539	1038	1047	1056	rVB2	352367	646101	18.49%	5.647%
5	11.184	1320	1327	1335	rVB	135135	251458	7.19%	2.198%
6	13.593	1730	1737	1744	rVB	1031386	1612912	46.15%	14.098%
7	14.968	1964	1971	1978	rBV	207247	349312	9.99%	3.053%
8	16.454	2214	2224	2230	rBV	966161	1514593	43.34%	13.239%
9	17.718	2433	2439	2445	rVB	328282	492435	14.09%	4.304%
10	20.291	2871	2877	2884	rVB	2715507	3494951	100.00%	30.548%
11	22.042	3168	3175	3182	rVB2	295932	527504	15.09%	4.611%
12	25.626	3773	3785	3795	rBV	197273	658349	18.84%	5.754%




Sum of corrected areas: 11440802

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059736.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

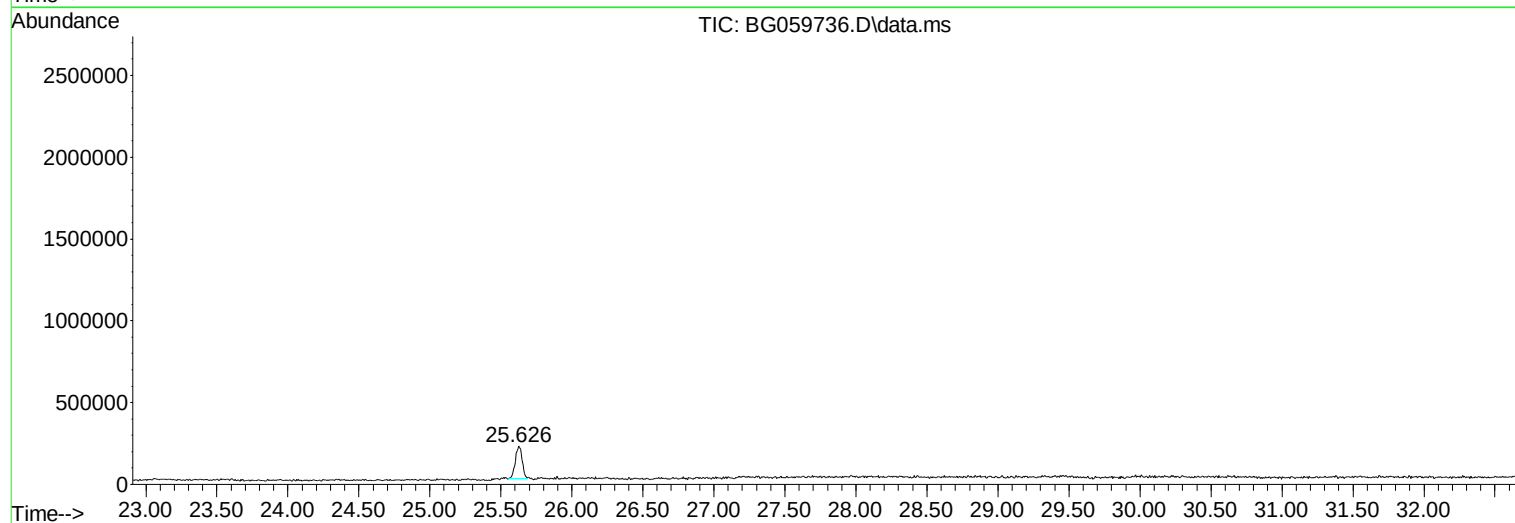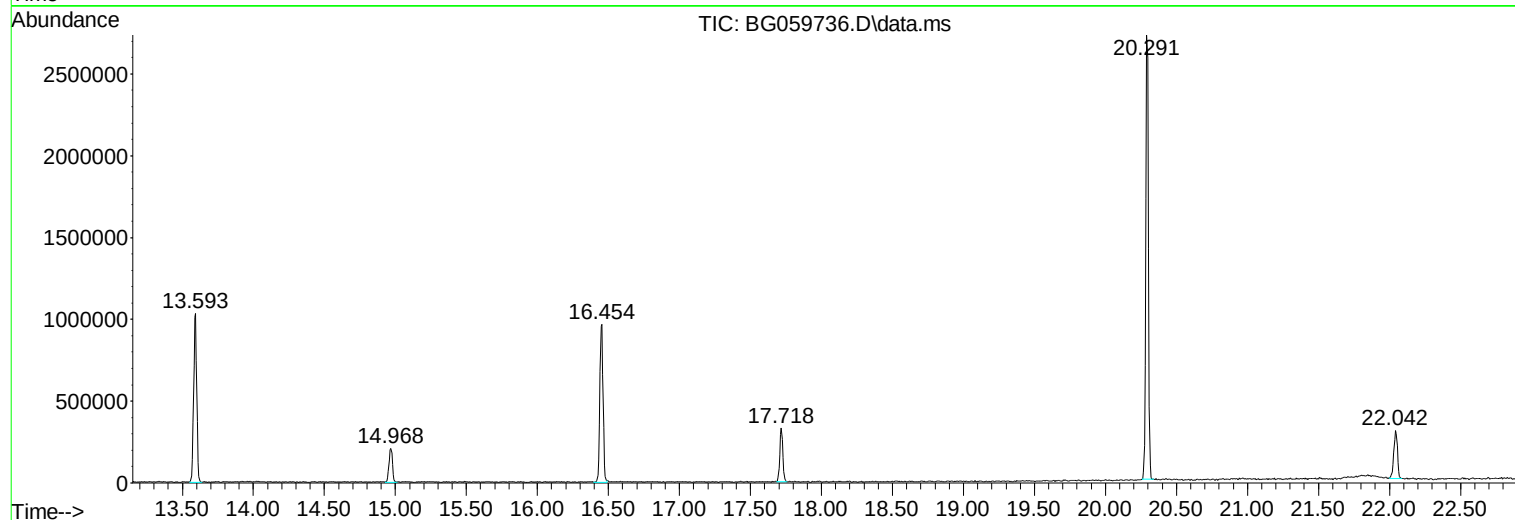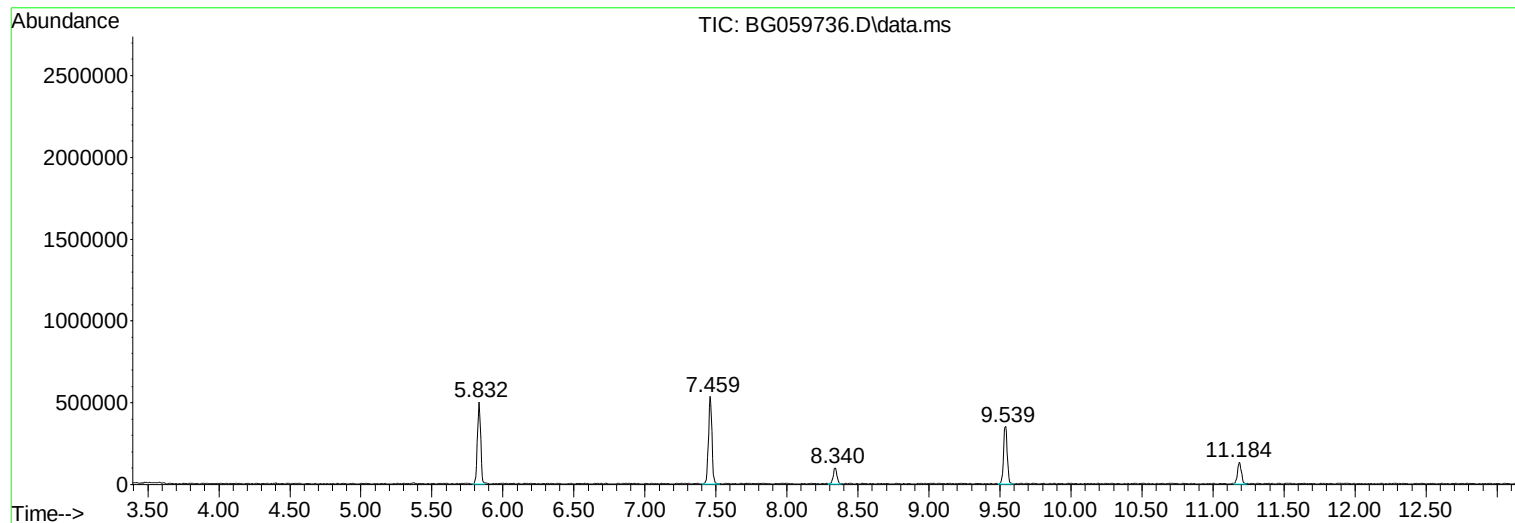

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059736.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected
