

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059752.D
Acq On : 18 Nov 2023 6:30
Operator : MA/JU
Sample : PB157152TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157152TB

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.832	407	416	424	rBV	417224	666008	15.67%	5.921%
2	7.460	684	693	700	rBV	472306	796331	18.73%	7.080%
3	8.335	837	842	848	rBV2	82349	137591	3.24%	1.223%
4	9.540	1040	1047	1054	rBV	296108	521670	12.27%	4.638%
5	11.185	1320	1327	1335	rVB2	103914	197123	4.64%	1.753%
6	13.588	1729	1736	1743	rBV	890706	1356922	31.92%	12.064%
7	14.969	1965	1971	1976	rVB2	189616	278855	6.56%	2.479%
8	16.449	2216	2223	2234	rBV	822867	1272612	29.94%	11.315%
9	17.718	2428	2439	2445	rBV	286638	442496	10.41%	3.934%
10	20.292	2870	2877	2884	rBV	3429991	4250676	100.00%	37.793%
11	22.043	3168	3175	3183	rVB2	368001	636660	14.98%	5.661%
12	25.621	3770	3784	3797	rBV2	217950	690369	16.24%	6.138%




Sum of corrected areas: 11247313

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059752.D
Acq On : 18 Nov 2023 6:30
Operator : MA/JU
Sample : PB157152TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157152TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

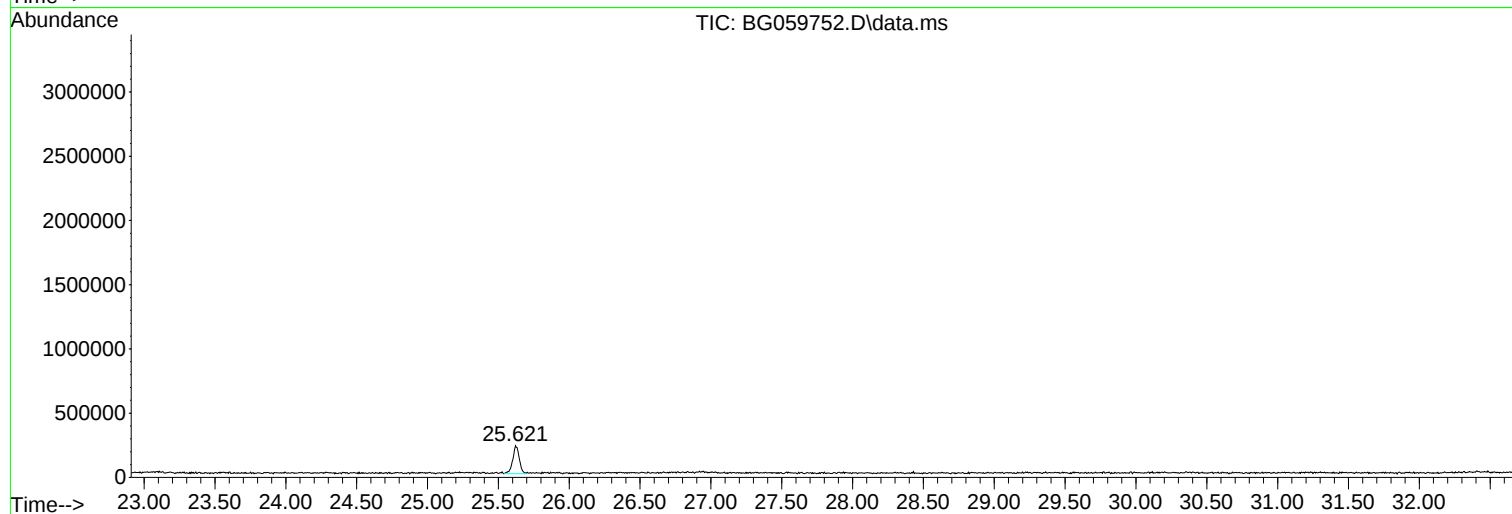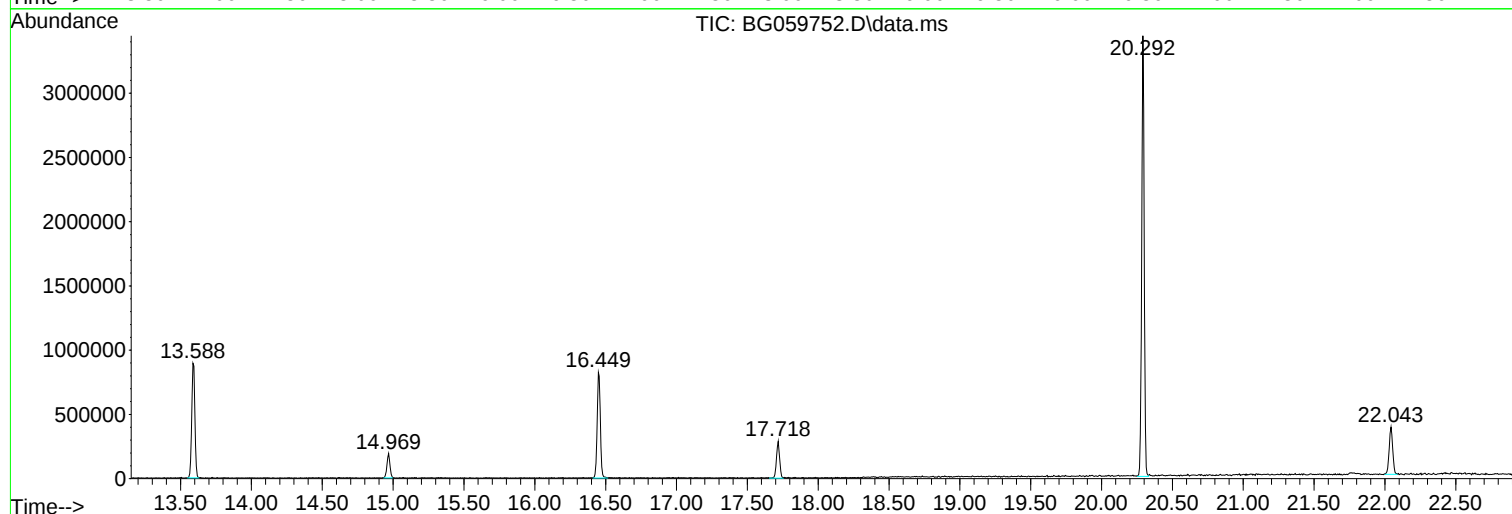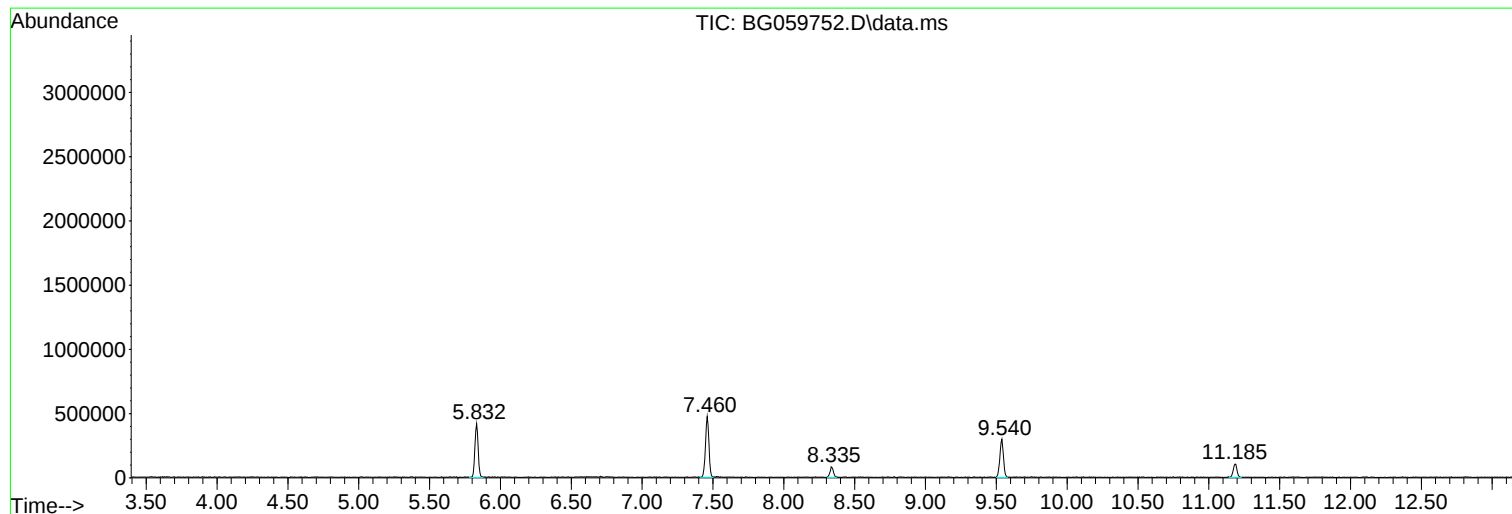

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059752.D
Acq On : 18 Nov 2023 6:30
Operator : MA/JU
Sample : PB157152TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157152TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059752.D
Acq On : 18 Nov 2023 6:30
Operator : MA/JU
Sample : PB157152TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157152TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------