

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
 Data File : BG059763.D
 Acq On : 18 Nov 2023 13:52
 Operator : MA/JU
 Sample : 05384-01 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EO-01-11102023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.565	367	370	375	rVB	4925	7457	1.09%	0.135%
2	5.835	408	416	422	rBV	86780	139549	20.44%	2.528%
3	6.058	448	454	459	rBV	7124	13677	2.00%	0.248%
4	6.563	537	540	543	rVB4	8893	9500	1.39%	0.172%
5	7.457	687	692	703	rVB2	100448	175583	25.72%	3.181%
6	8.214	816	821	823	rBV2	5026	7831	1.15%	0.142%
7	8.344	834	843	850	rBV	142570	243727	35.71%	4.416%
8	9.542	1037	1047	1055	rBV	73021	130196	19.07%	2.359%
9	11.187	1319	1327	1335	rBV	177667	322472	47.24%	5.843%
10	11.846	1436	1439	1446	rVB	6429	7643	1.12%	0.138%
11	12.815	1601	1604	1608	rBV3	4797	8022	1.18%	0.145%
12	12.921	1618	1622	1624	rBV2	6079	10445	1.53%	0.189%
13	12.962	1626	1629	1631	rBV	8010	8330	1.22%	0.151%
14	13.044	1639	1643	1644	rBV3	11313	13531	1.98%	0.245%
15	13.109	1652	1654	1657	rVB2	8876	9185	1.35%	0.166%
16	13.285	1681	1684	1686	rBV2	11104	13494	1.98%	0.244%
17	13.408	1702	1705	1708	rBV4	8064	11723	1.72%	0.212%
18	13.485	1714	1718	1721	rBV3	13261	16765	2.46%	0.304%
19	13.591	1730	1736	1743	rBV	307190	489451	71.71%	8.868%
20	13.643	1743	1745	1746	rBV	13421	6928	1.01%	0.126%
21	13.714	1754	1757	1763	rVB7	15233	23624	3.46%	0.428%
22	14.207	1839	1841	1842	rBV3	9104	6981	1.02%	0.126%
23	14.290	1853	1855	1857	rVB2	13044	7661	1.12%	0.139%
24	14.395	1871	1873	1877	rVB4	7217	8446	1.24%	0.153%
25	14.454	1882	1883	1886	rVB3	12607	7862	1.15%	0.142%
26	14.478	1886	1887	1889	rVB2	10630	7181	1.05%	0.130%
27	14.495	1889	1890	1891	rBV	12891	6984	1.02%	0.127%
28	14.760	1932	1935	1936	rBV	12447	12491	1.83%	0.226%
29	14.783	1936	1939	1942	rVB4	14091	21328	3.12%	0.386%
30	14.901	1957	1959	1962	rBV4	6799	8890	1.30%	0.161%
31	14.971	1964	1971	1979	rBV2	405201	647317	94.84%	11.728%
32	15.071	1986	1988	1991	rBV4	8180	10674	1.56%	0.193%
33	15.171	2002	2005	2008	rVB4	8242	9875	1.45%	0.179%
34	15.259	2017	2020	2023	rBV5	6308	8660	1.27%	0.157%
35	15.336	2031	2033	2036	rVB4	13642	12807	1.88%	0.232%
36	15.359	2036	2037	2038	rBV	13953	7167	1.05%	0.130%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
 Data File : BG059763.D
 Acq On : 18 Nov 2023 13:52
 Operator : MA/JU
 Sample : 05384-01 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EO-01-11102023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.612	2079	2080	2082	rVB2	10671	7122	1.04%	0.129%
38	15.688	2090	2093	2095	rVB4	7957	8459	1.24%	0.153%
39	15.723	2097	2099	2104	rVB5	20756	23049	3.38%	0.418%
40	15.823	2113	2116	2121	rVB6	18994	40218	5.89%	0.729%
41	15.888	2125	2127	2132	rVB5	4752	7365	1.08%	0.133%
42	15.941	2135	2136	2139	rBV3	8112	8416	1.23%	0.152%
43	16.229	2183	2185	2186	rVB2	12480	8145	1.19%	0.148%
44	16.240	2186	2187	2190	rBV3	12581	14861	2.18%	0.269%
45	16.375	2206	2210	2212	rVV4	11653	14646	2.15%	0.265%
46	16.452	2216	2223	2230	rBV3	221946	351247	51.46%	6.364%
47	16.563	2240	2242	2243	rBV2	11503	8657	1.27%	0.157%
48	16.581	2243	2245	2254	rVV10	26916	54895	8.04%	0.995%
49	16.704	2264	2266	2268	rBV3	10915	10134	1.48%	0.184%
50	16.728	2268	2270	2273	rVV4	11017	10474	1.53%	0.190%
51	16.769	2276	2277	2279	rBV2	7740	6971	1.02%	0.126%
52	16.904	2297	2300	2303	rBV5	12095	18309	2.68%	0.332%
53	17.239	2355	2357	2358	rBV2	8124	6981	1.02%	0.126%
54	17.286	2363	2365	2367	rVB3	10699	8669	1.27%	0.157%
55	17.380	2378	2381	2385	rVB5	27272	29074	4.26%	0.527%
56	17.427	2387	2389	2390	rVV2	11786	7750	1.14%	0.140%
57	17.539	2406	2408	2411	rBV3	11851	13777	2.02%	0.250%
58	17.609	2417	2420	2421	rBV3	10190	9155	1.34%	0.166%
59	17.721	2434	2439	2444	rBV	454087	682571	100.00%	12.367%
60	17.762	2444	2446	2452	rVB2	64766	91776	13.45%	1.663%
61	18.121	2502	2507	2509	rBV6	24247	32882	4.82%	0.596%
62	18.191	2517	2519	2522	rVB4	13249	11424	1.67%	0.207%
63	18.215	2522	2523	2525	rBV2	11654	10463	1.53%	0.190%
64	18.391	2552	2553	2554	rBV	23822	12761	1.87%	0.231%
65	18.426	2556	2559	2560	rVV3	16207	15151	2.22%	0.275%
66	18.526	2574	2576	2581	rVB5	39275	48975	7.18%	0.887%
67	18.632	2592	2594	2597	rVB3	25654	28574	4.19%	0.518%
68	19.008	2657	2658	2659	rBV	22892	14542	2.13%	0.263%
69	19.061	2665	2667	2671	rBV5	19558	30365	4.45%	0.550%
70	19.301	2706	2708	2711	rVB4	19253	14619	2.14%	0.265%
71	19.754	2782	2785	2790	rBV2	85967	102228	14.98%	1.852%
72	20.001	2825	2827	2831	rBV5	47936	55033	8.06%	0.997%
73	20.118	2844	2847	2852	rVB2	117468	161279	23.63%	2.922%
74	20.294	2873	2877	2882	rVB	432060	537665	78.77%	9.741%
75	22.045	3170	3175	3181	rBV2	297775	547219	80.17%	9.915%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059763.D
Acq On : 18 Nov 2023 13:52
Operator : MA/JU
Sample : 05384-01 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EO-01-11102023

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 5519358

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059763.D
Acq On : 18 Nov 2023 13:52
Operator : MA/JU
Sample : 05384-01 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EO-01-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

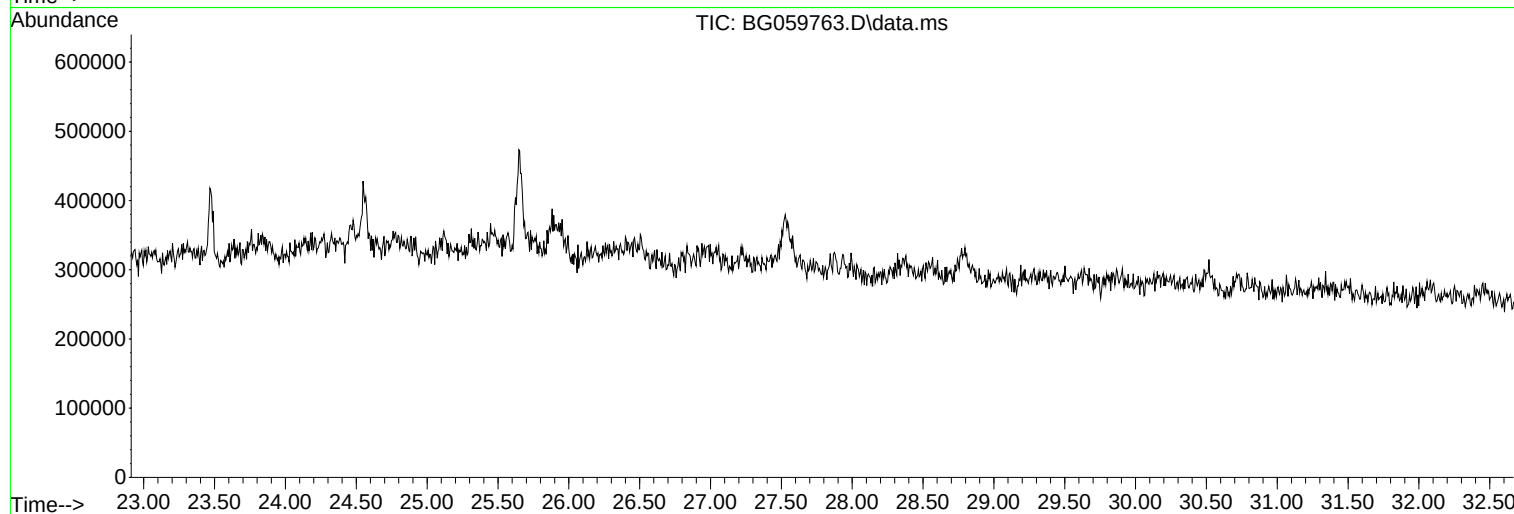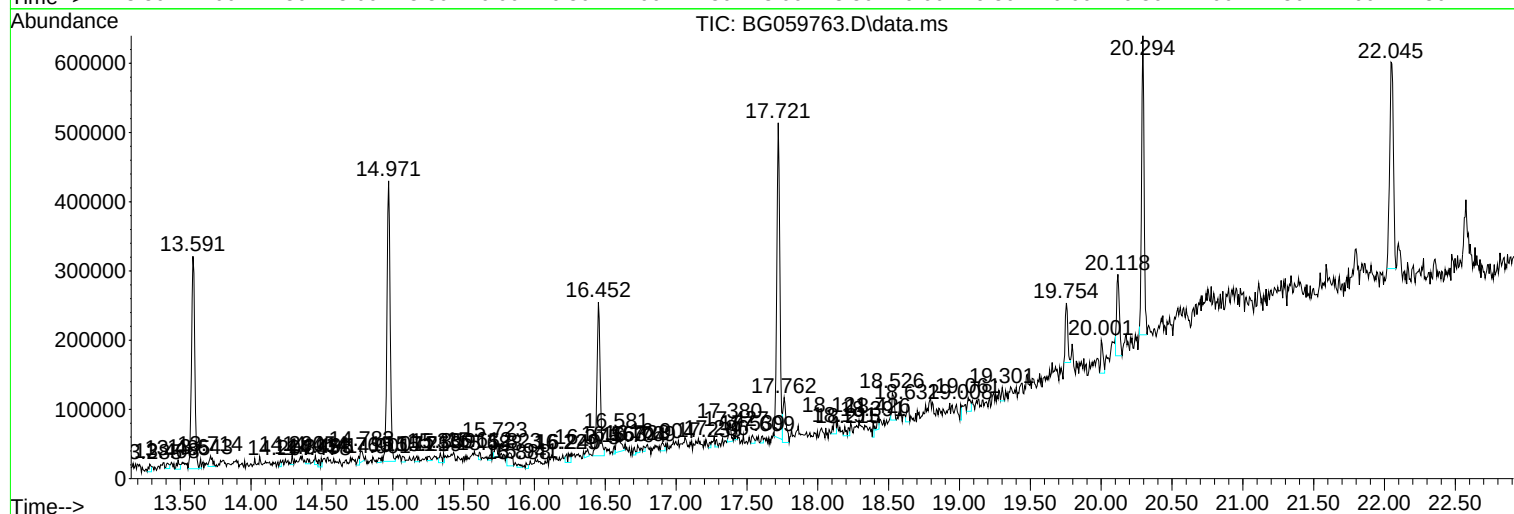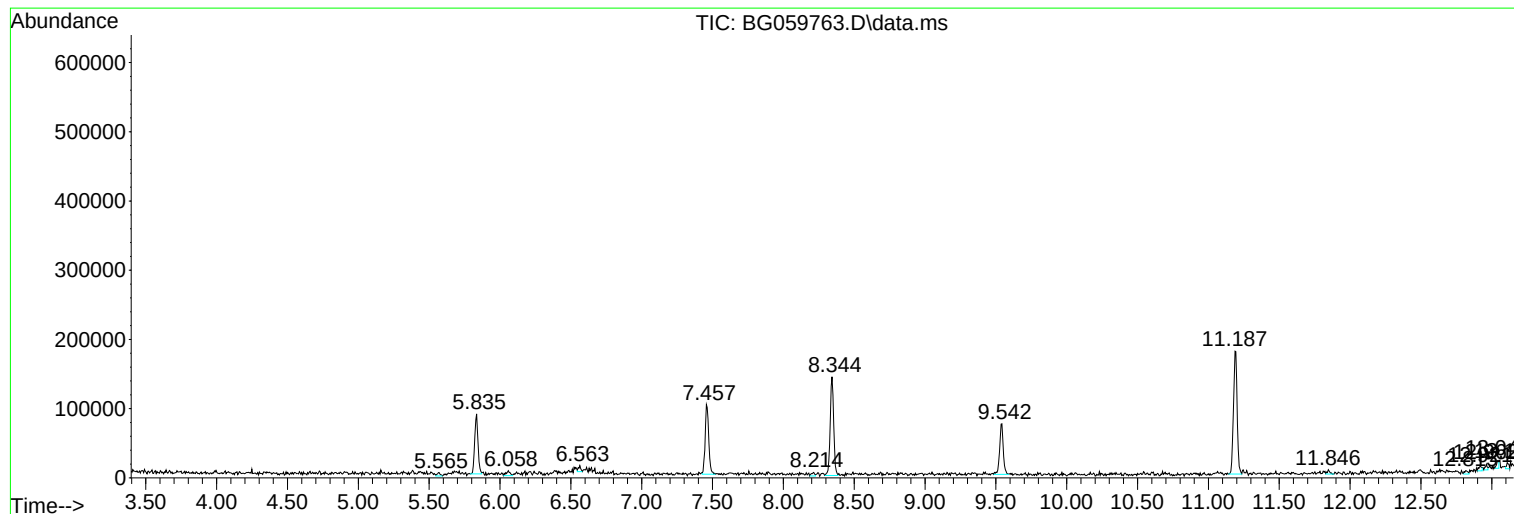

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059763.D
Acq On : 18 Nov 2023 13:52
Operator : MA/JU
Sample : 05384-01 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EO-01-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059763.D
Acq On : 18 Nov 2023 13:52
Operator : MA/JU
Sample : 05384-01 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EO-01-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------