

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
 Data File : BG059765.D
 Acq On : 18 Nov 2023 15:13
 Operator : MA/JU
 Sample : 05385-03 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HR-03-11102023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.506	19	20	23	rVB2	9963	8001	1.10%	0.162%
2	3.571	28	31	34	rVB3	7663	9894	1.37%	0.201%
3	4.182	134	135	140	rBV2	9511	12559	1.73%	0.255%
4	4.781	234	237	239	rBV2	9204	12198	1.68%	0.247%
5	4.828	244	245	250	rVB2	10852	13799	1.91%	0.280%
6	5.327	327	330	332	rBV2	6209	7979	1.10%	0.162%
7	5.521	361	363	365	rVB2	8467	7460	1.03%	0.151%
8	5.839	411	417	422	rBV2	87183	139967	19.32%	2.840%
9	6.538	533	536	538	rVB2	8199	7505	1.04%	0.152%
10	7.460	687	693	699	rBV	101442	172677	23.84%	3.503%
11	7.537	705	706	712	rVB	4439	7380	1.02%	0.150%
12	8.342	837	843	851	rBV	154447	263578	36.39%	5.348%
13	9.305	1003	1007	1010	rVB	5197	8361	1.15%	0.170%
14	9.540	1038	1047	1053	rBV2	73077	134041	18.51%	2.719%
15	11.191	1320	1328	1336	rBV2	201344	369937	51.08%	7.505%
16	12.096	1480	1482	1486	rVB	5982	7661	1.06%	0.155%
17	12.166	1491	1494	1499	rVB3	5395	8525	1.18%	0.173%
18	12.378	1527	1530	1534	rBV2	6593	8306	1.15%	0.169%
19	12.707	1585	1586	1591	rVB2	8806	9037	1.25%	0.183%
20	13.042	1641	1643	1648	rVB3	8151	10394	1.44%	0.211%
21	13.089	1648	1651	1654	rBV	8996	11431	1.58%	0.232%
22	13.594	1731	1737	1744	rVB	320733	475080	65.59%	9.639%
23	13.688	1750	1753	1755	rVB3	6822	7368	1.02%	0.149%
24	13.712	1755	1757	1761	rVB3	6912	8476	1.17%	0.172%
25	14.011	1805	1808	1810	rVB4	7572	7295	1.01%	0.148%
26	14.323	1859	1861	1863	rBV2	9632	7326	1.01%	0.149%
27	14.358	1863	1867	1871	rVV6	10196	19159	2.65%	0.389%
28	14.669	1918	1920	1921	rBV2	8196	7395	1.02%	0.150%
29	14.711	1925	1927	1932	rVB6	5888	8333	1.15%	0.169%
30	14.969	1963	1971	1979	rBV	423892	653334	90.20%	13.255%
31	15.075	1987	1989	1992	rBV4	9822	11925	1.65%	0.242%
32	15.357	2035	2037	2041	rBV4	6237	7788	1.08%	0.158%
33	15.557	2069	2071	2074	rBV4	8424	7694	1.06%	0.156%
34	15.698	2093	2095	2099	rVB5	11841	13907	1.92%	0.282%
35	16.050	2153	2155	2157	rBV3	11547	12386	1.71%	0.251%
36	16.121	2163	2167	2170	rBV5	8665	14872	2.05%	0.302%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
 Data File : BG059765.D
 Acq On : 18 Nov 2023 15:13
 Operator : MA/JU
 Sample : 05385-03 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HR-03-11102023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.456	2218	2224	2230	rVV4	195125	307384	42.44%	6.236%
38	16.538	2236	2238	2241	rBV4	7856	7713	1.06%	0.156%
39	16.591	2243	2247	2248	rBV4	8324	9531	1.32%	0.193%
40	16.608	2248	2250	2252	rVB3	10895	7481	1.03%	0.152%
41	16.796	2281	2282	2285	rVB3	15700	12263	1.69%	0.249%
42	16.943	2306	2307	2311	rBV4	11254	11626	1.61%	0.236%
43	16.984	2313	2314	2317	rVV3	11321	7803	1.08%	0.158%
44	17.008	2317	2318	2321	rVV3	9576	7600	1.05%	0.154%
45	17.284	2361	2365	2368	rBV6	13331	22209	3.07%	0.451%
46	17.419	2386	2388	2390	rBV3	16895	18567	2.56%	0.377%
47	17.496	2399	2401	2403	rBV3	8407	7512	1.04%	0.152%
48	17.625	2421	2423	2425	rVB3	13054	10635	1.47%	0.216%
49	17.678	2429	2432	2434	rBV4	12314	14000	1.93%	0.284%
50	17.725	2434	2440	2447	rBV	454963	724291	100.00%	14.695%
51	17.854	2461	2462	2465	rBV2	9947	11396	1.57%	0.231%
52	17.983	2482	2484	2487	rVB4	15162	15713	2.17%	0.319%
53	18.007	2487	2488	2490	rVB2	19735	7440	1.03%	0.151%
54	18.030	2490	2492	2494	rBV3	13389	15302	2.11%	0.310%
55	18.124	2506	2508	2510	rBV3	10400	7340	1.01%	0.149%
56	18.295	2535	2537	2538	rBV2	19318	14720	2.03%	0.299%
57	18.330	2542	2543	2547	rVV4	13225	13286	1.83%	0.270%
58	18.530	2574	2577	2582	rVB6	44169	63716	8.80%	1.293%
59	18.806	2622	2624	2628	rBV5	21541	22337	3.08%	0.453%
60	18.900	2637	2640	2644	rBV6	26895	32614	4.50%	0.662%
61	19.282	2703	2705	2706	rBV2	27332	22168	3.06%	0.450%
62	20.298	2873	2878	2885	rVB	398493	505240	69.76%	10.251%
63	22.055	3171	3177	3184	rBV	304726	535989	74.00%	10.874%




Sum of corrected areas: 4928904

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059765.D
Acq On : 18 Nov 2023 15:13
Operator : MA/JU
Sample : 05385-03 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HR-03-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

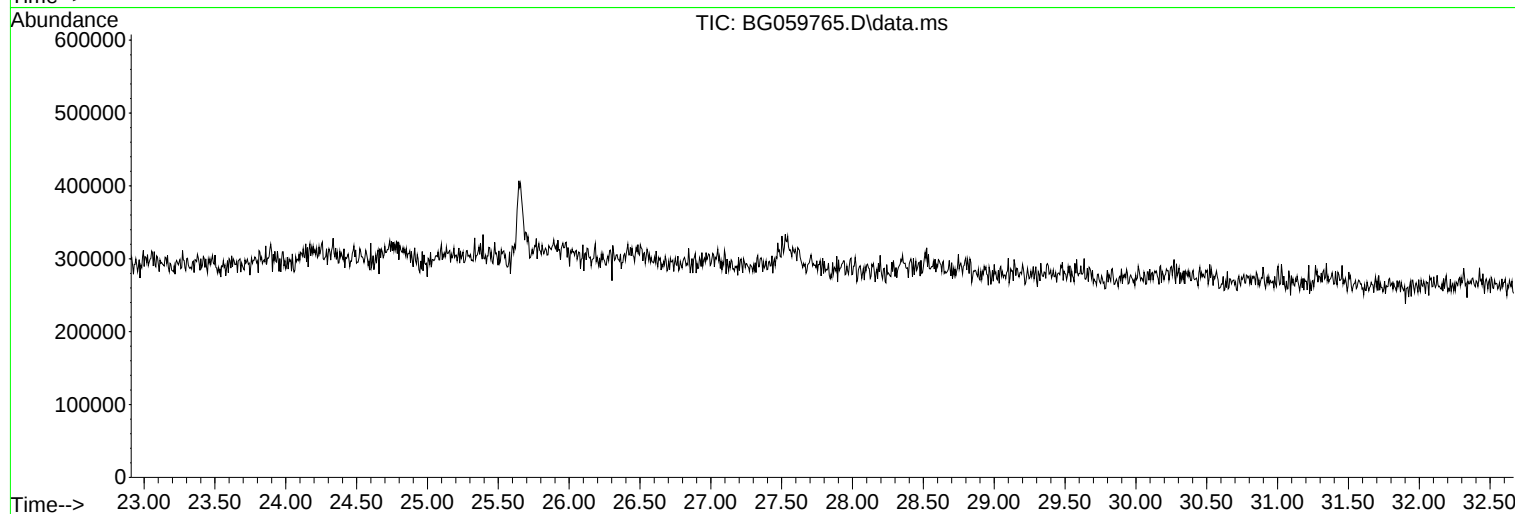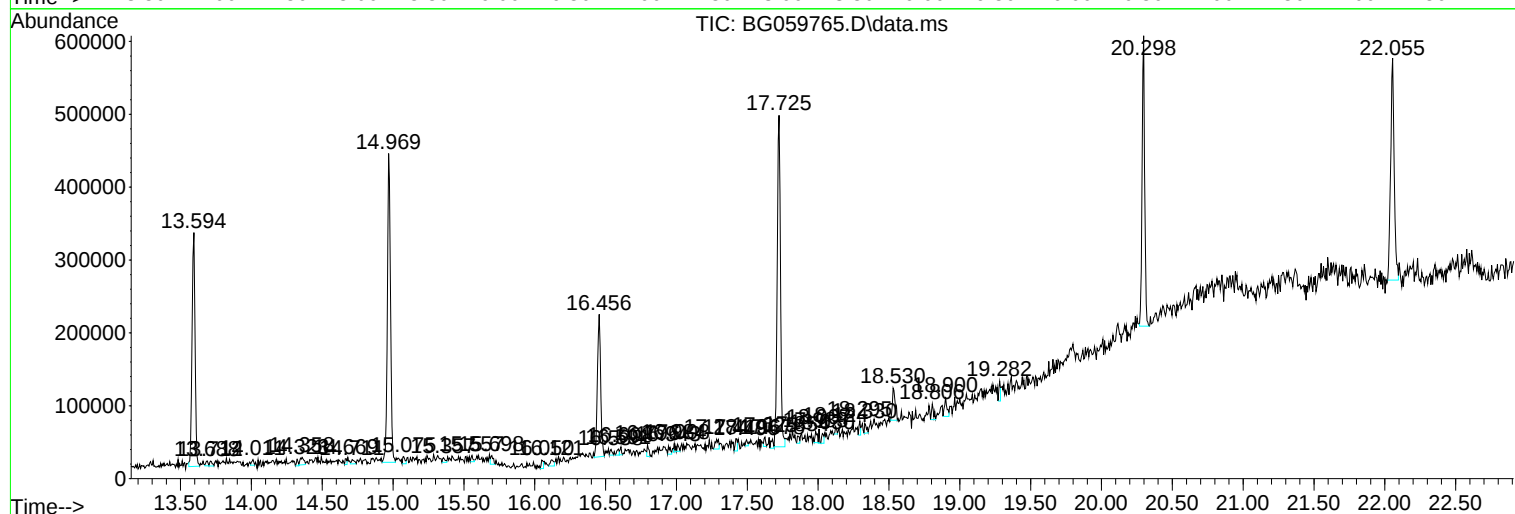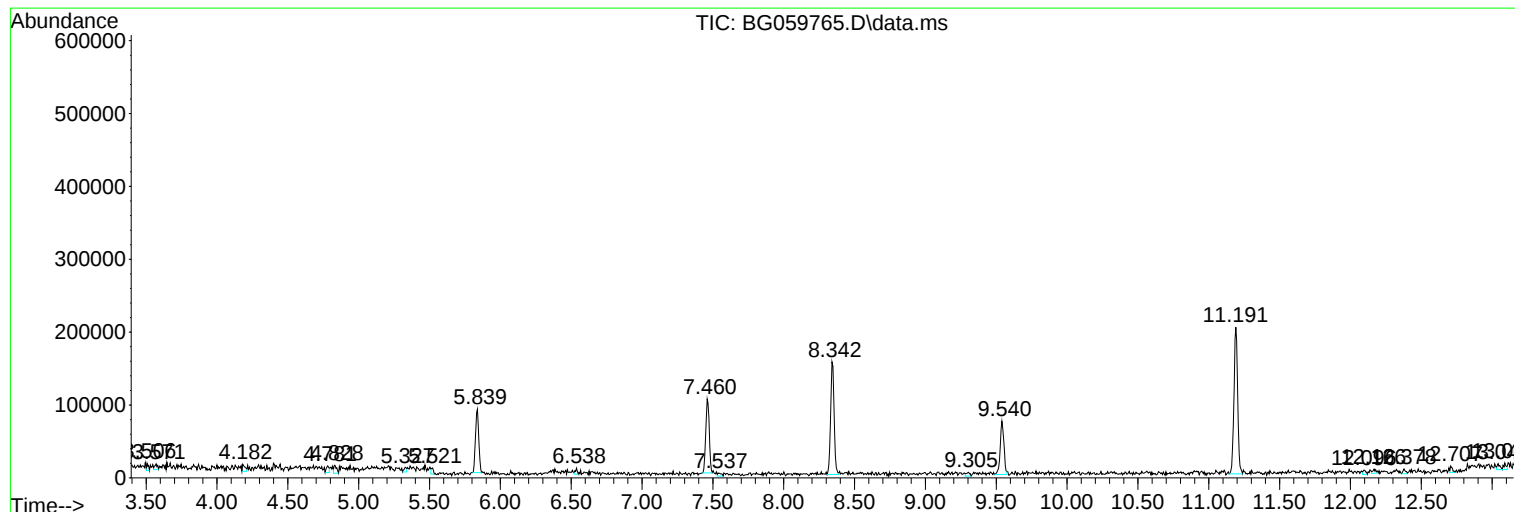

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059765.D
Acq On : 18 Nov 2023 15:13
Operator : MA/JU
Sample : 05385-03 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HR-03-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059765.D
Acq On : 18 Nov 2023 15:13
Operator : MA/JU
Sample : 05385-03 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HR-03-11102023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------