
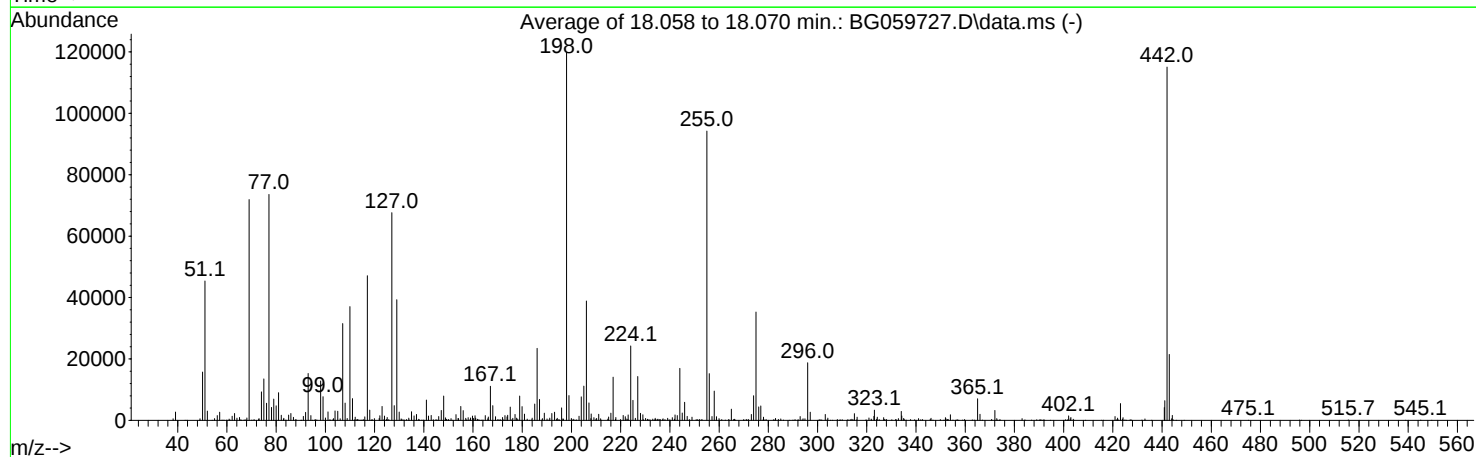


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059727.D
Acq On : 17 Nov 2023 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 17 01:51:38 2023

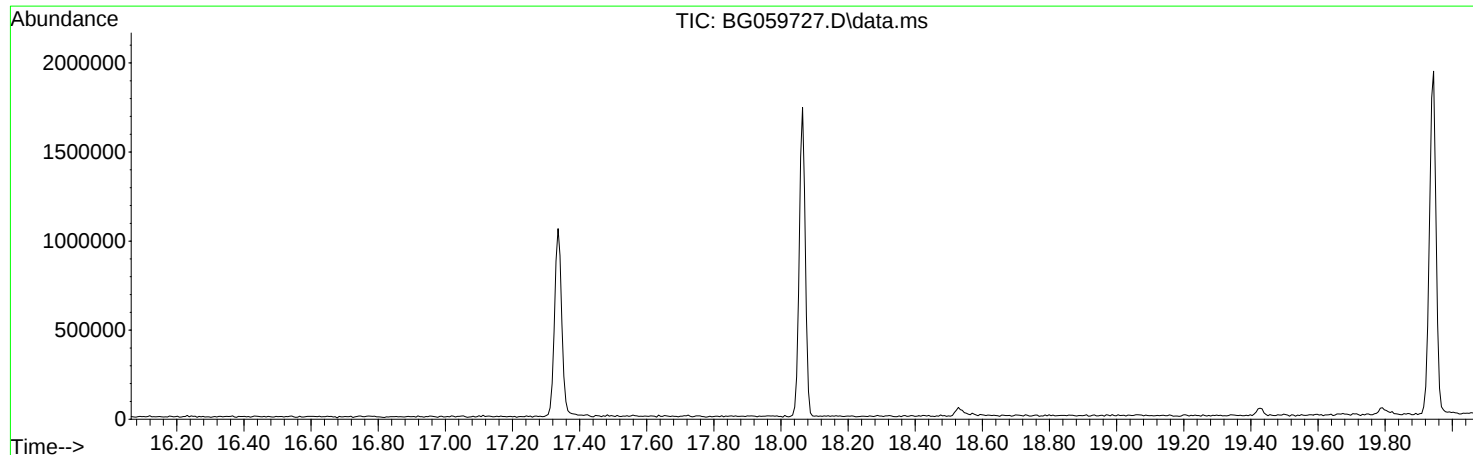




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	37.9	45397	PASS
68	69	0.00	2	1.1	805	PASS
69	198	0.00	100	60.0	71915	PASS
70	69	0.00	2	0.2	128	PASS
127	198	10	80	56.5	67669	PASS
197	198	0.00	2	0.3	411	PASS
198	198	100	100	100.0	119816	PASS
199	198	5	9	6.7	8087	PASS
275	198	10	60	29.5	35299	PASS
365	198	1	100	5.9	7063	PASS
441	198	0.01	100	5.4	6411	PASS
442	442	50	100	100.0	115080	PASS
443	442	15	24	18.7	21483	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059727.D
Acq On : 17 Nov 2023 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 13:45:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

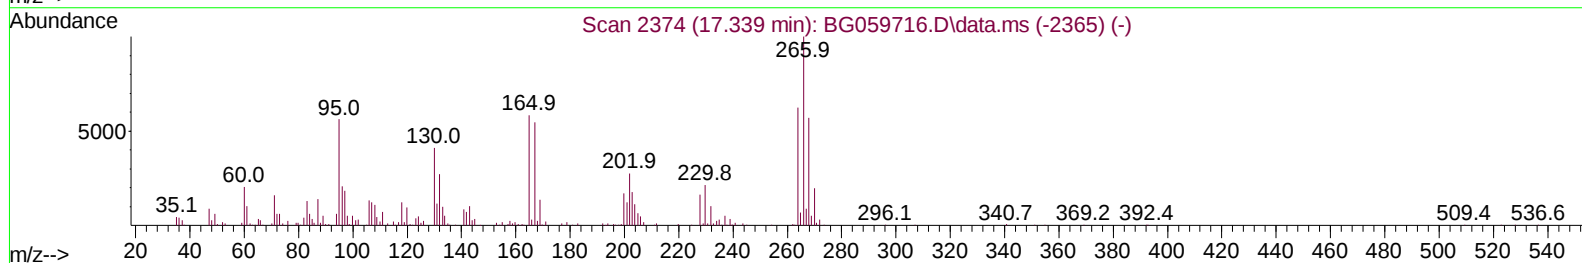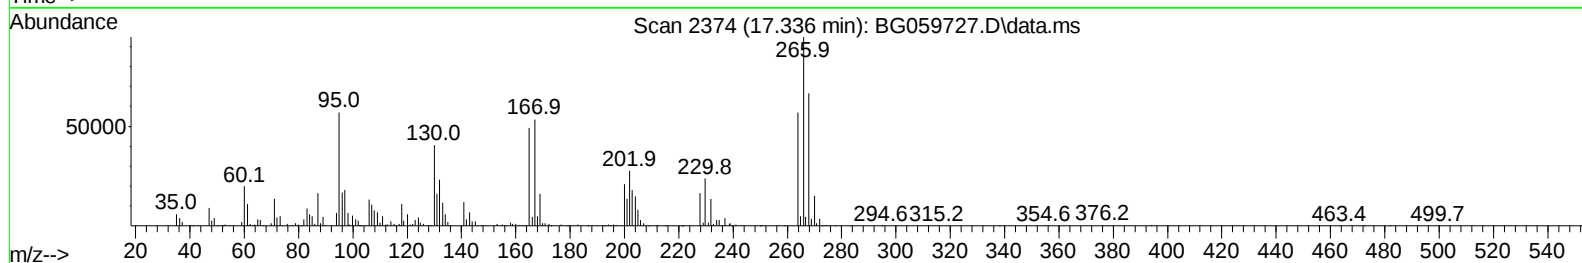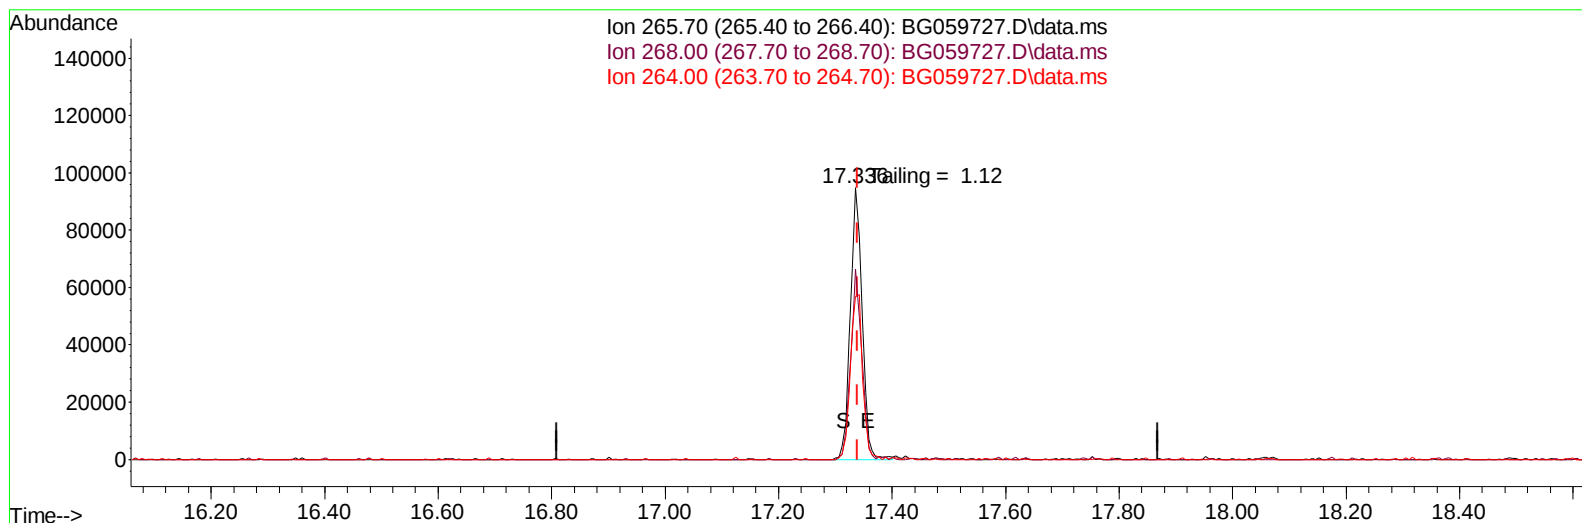

TIC: BG059727.D\data.ms

(70) Pentachlorophenol (C)

17.336min (-0.003) 140483.76 ng




response 135406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	70.21#
264.00	62.30	60.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059727.D
Acq On : 17 Nov 2023 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 13:45:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

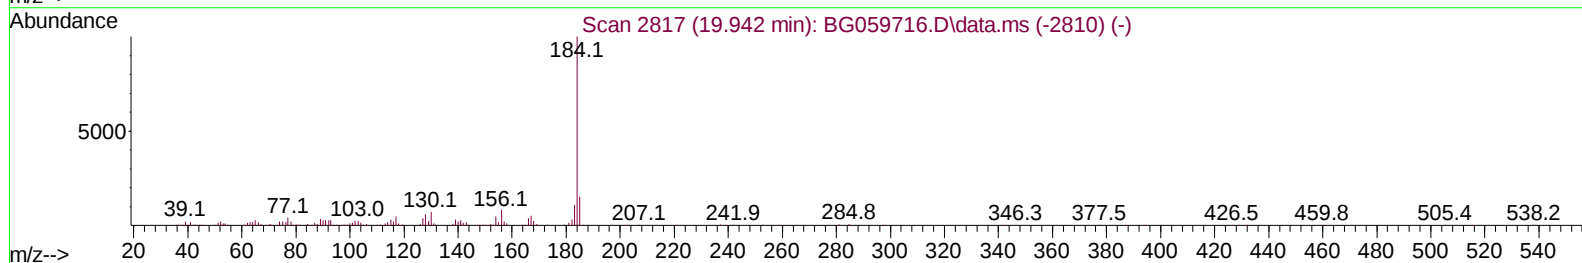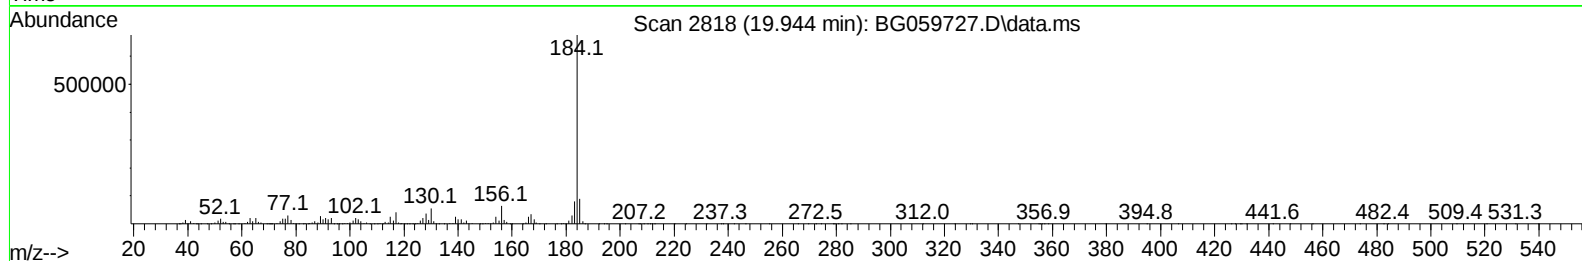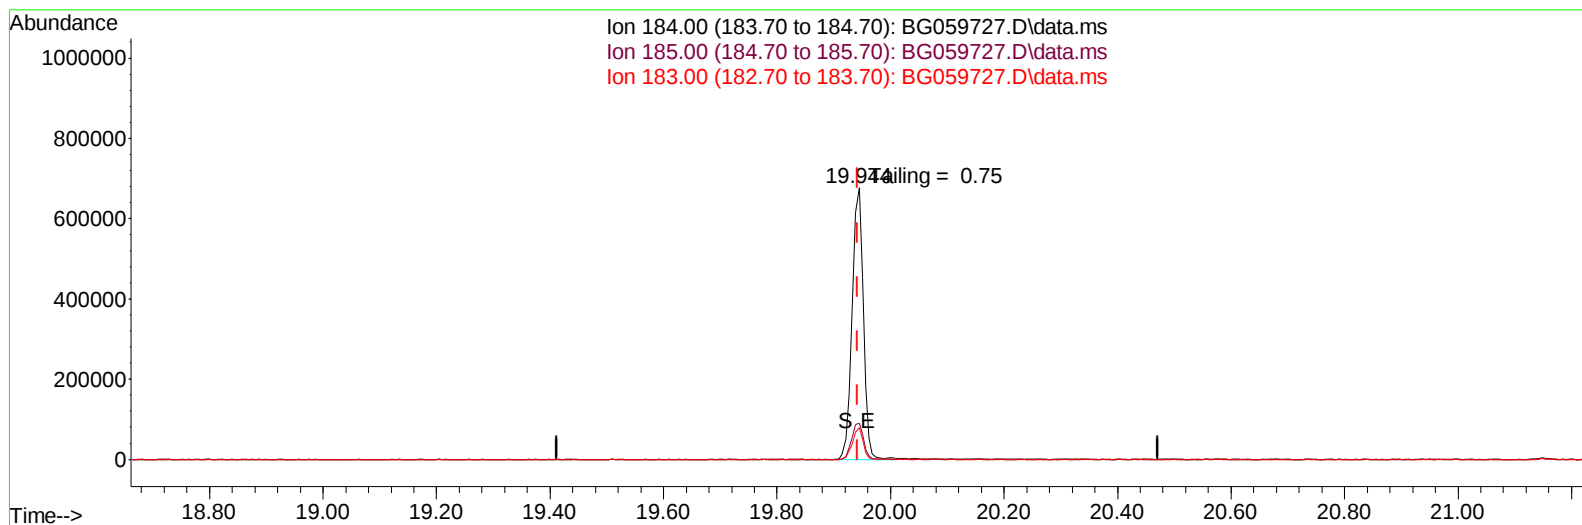

TIC: BG059727.D\data.ms

(77) Benzidine

19.944min (+ 0.003) 236651.43 ng

response 922995

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.41
183.00	11.00	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2023	BNA_G	<u>BG059727.D</u>
Compound Name	Response	Retention Time
DDT	384399	21.155
DDD	11944	20.696
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11944	396343	3.01

Instrument :
BNA_G
ClientSampleId :
DFTPP