
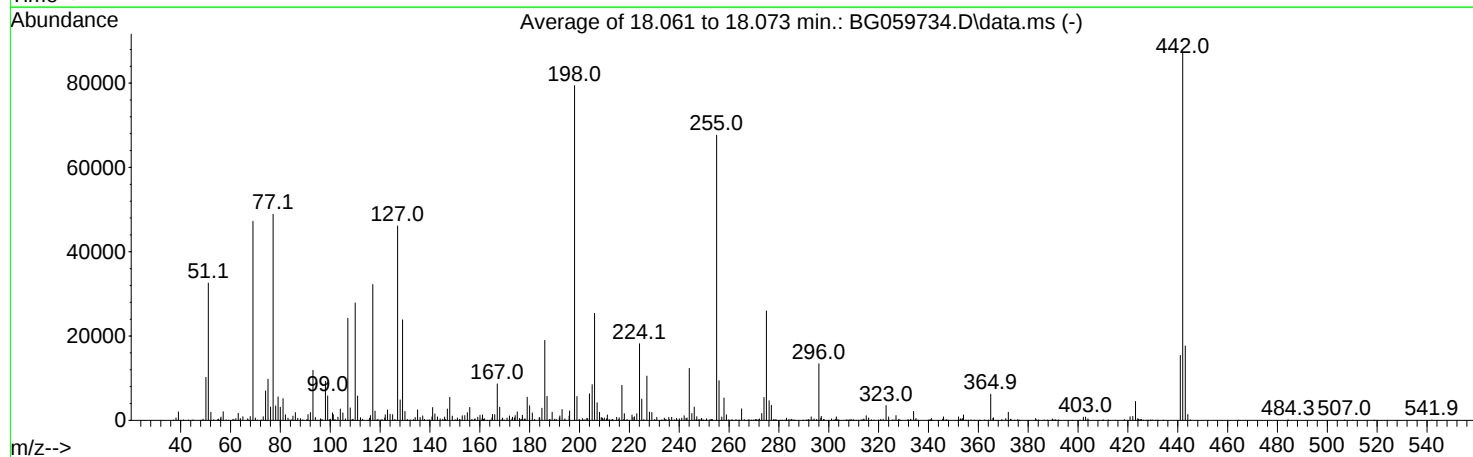


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
 Data File : BG059734.D
 Acq On : 17 Nov 2023 16:46
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 01:51:38 2023

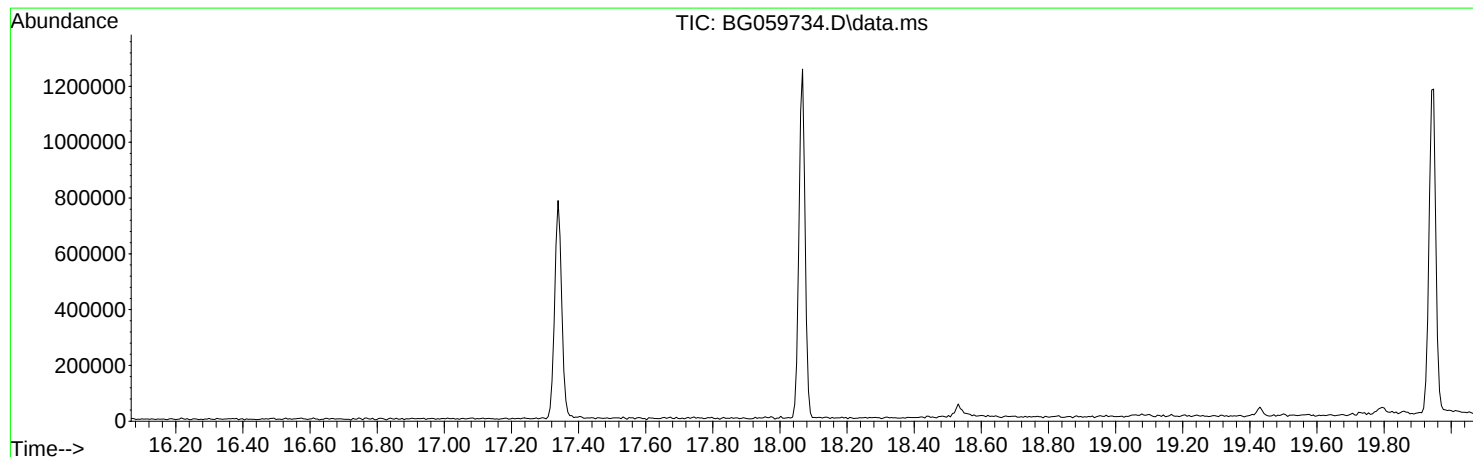




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	32576	PASS
68	69	0.00	2	1.9	919	PASS
69	198	0.00	100	59.5	47219	PASS
70	69	0.00	2	1.2	571	PASS
127	198	10	80	58.1	46111	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79389	PASS
199	198	5	9	7.1	5673	PASS
275	198	10	60	32.7	25944	PASS
365	198	1	100	7.8	6203	PASS
441	198	0.01	100	19.4	15415	PASS
442	442	50	100	100.0	87264	PASS
443	442	15	24	20.2	17658	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059734.D
Acq On : 17 Nov 2023 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 17:32:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

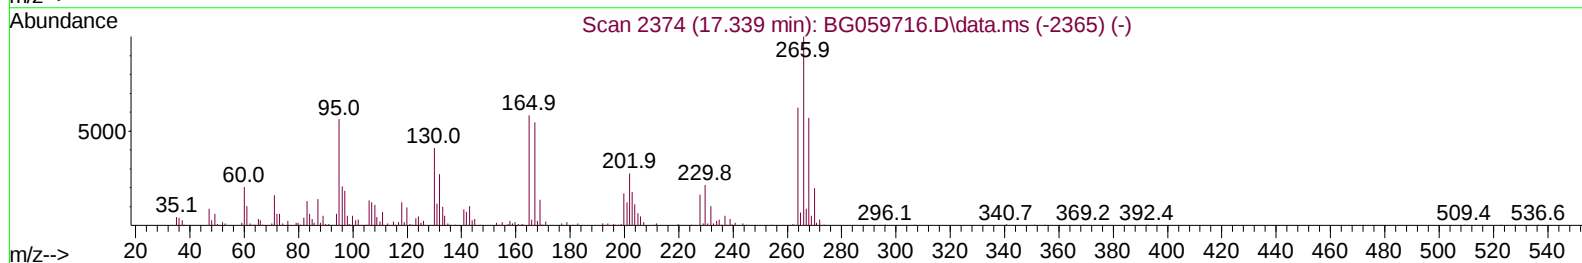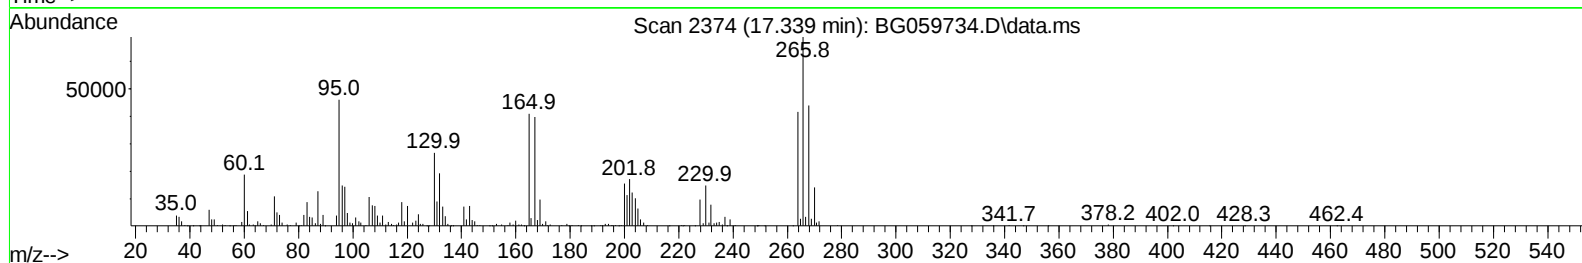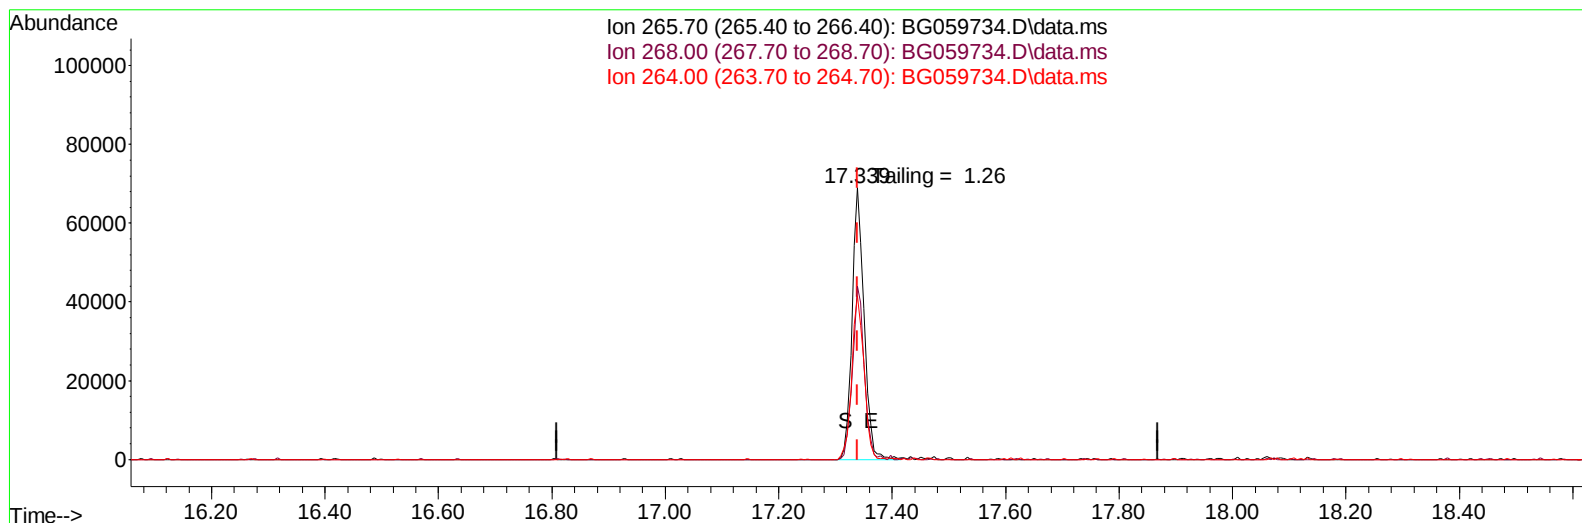

TIC: BG059734.D\data.ms

(70) Pentachlorophenol (C)

17.339min (-0.000) 95398.24 ng




response 101437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	63.85
264.00	62.30	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059734.D
Acq On : 17 Nov 2023 16:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 17:32:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

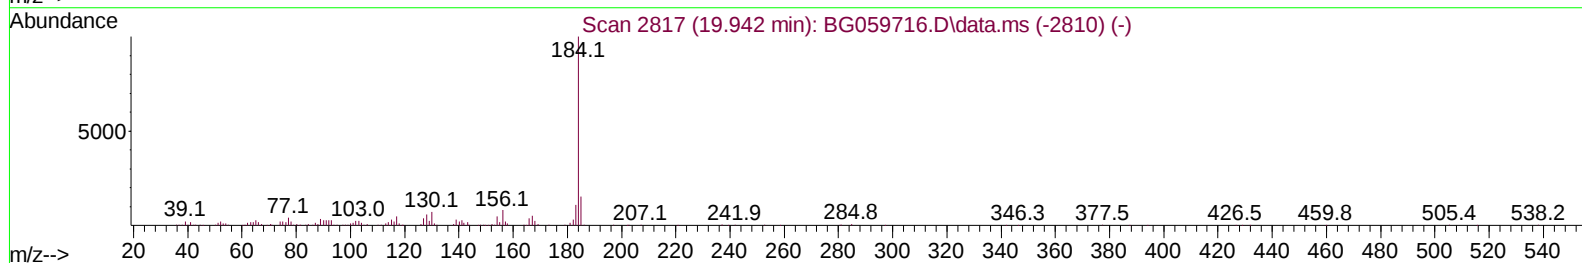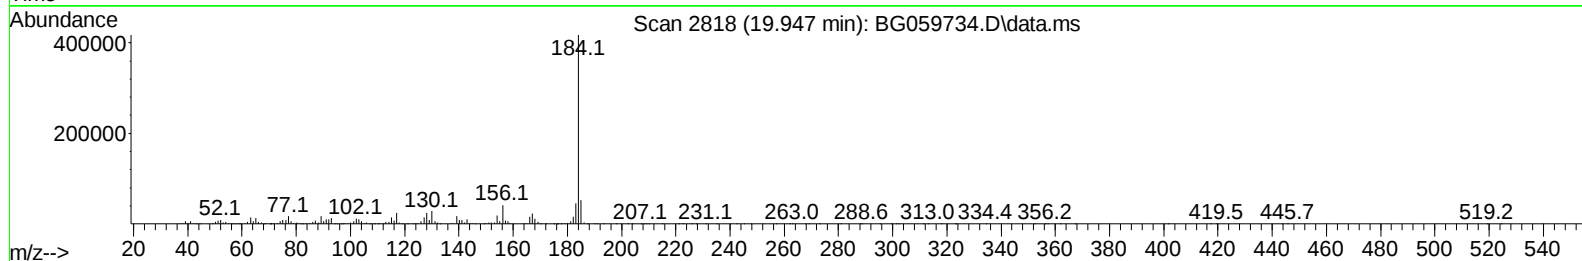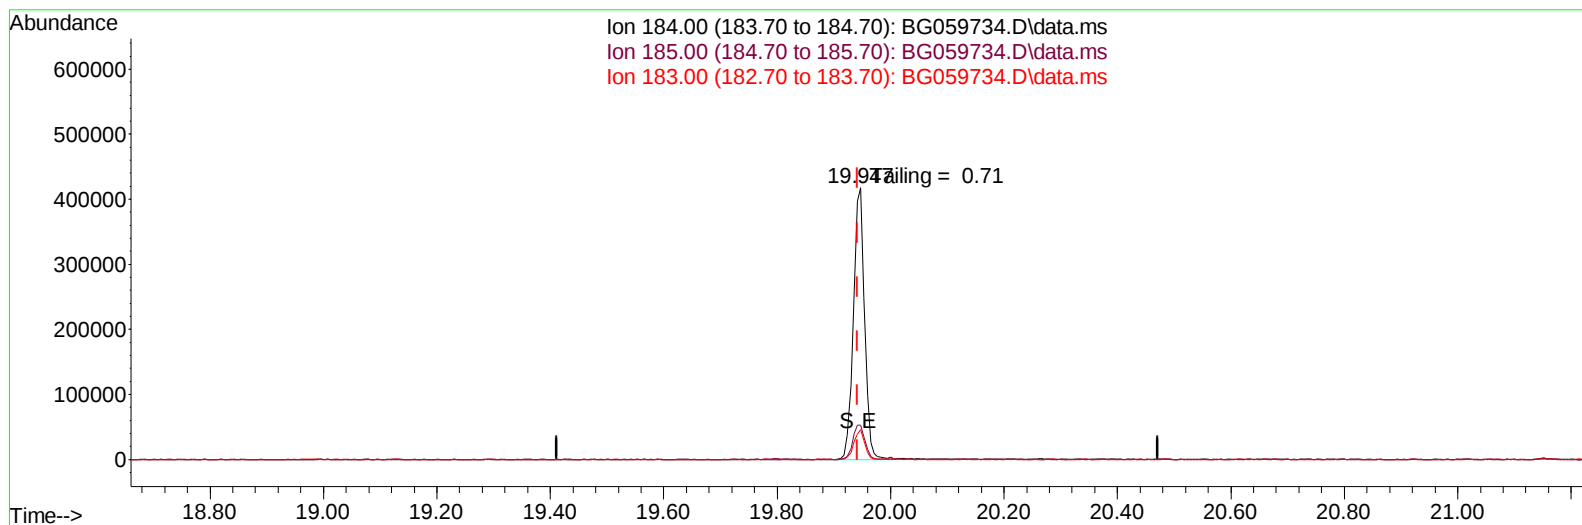

TIC: BG059734.D\data.ms

(77) Benzidine

19.947min (+ 0.006) 385881.36 ng

response 577510

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	12.55
183.00	11.00	11.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2023	BNA_G	<u>BG059734.D</u>
Compound Name	Response	Retention Time
DDT	235481	21.158
DDD	6479	20.746
DDE		20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6479	241960	2.68

Instrument :
BNA_G
ClientSampleId :
DFTPP