
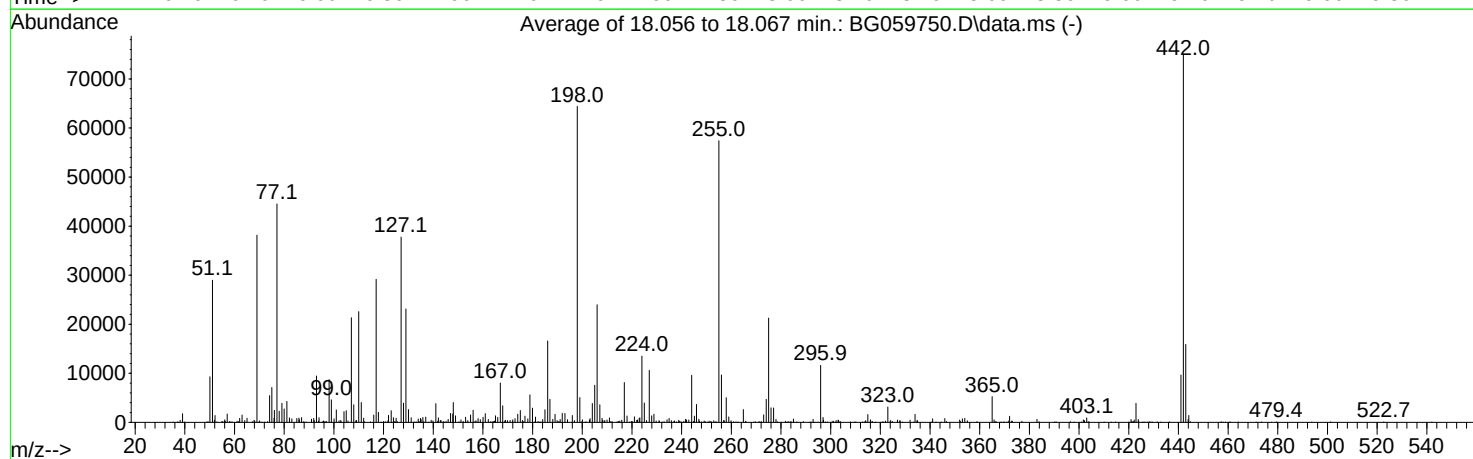


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059750.D
Acq On : 18 Nov 2023 5:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 17 01:51:38 2023

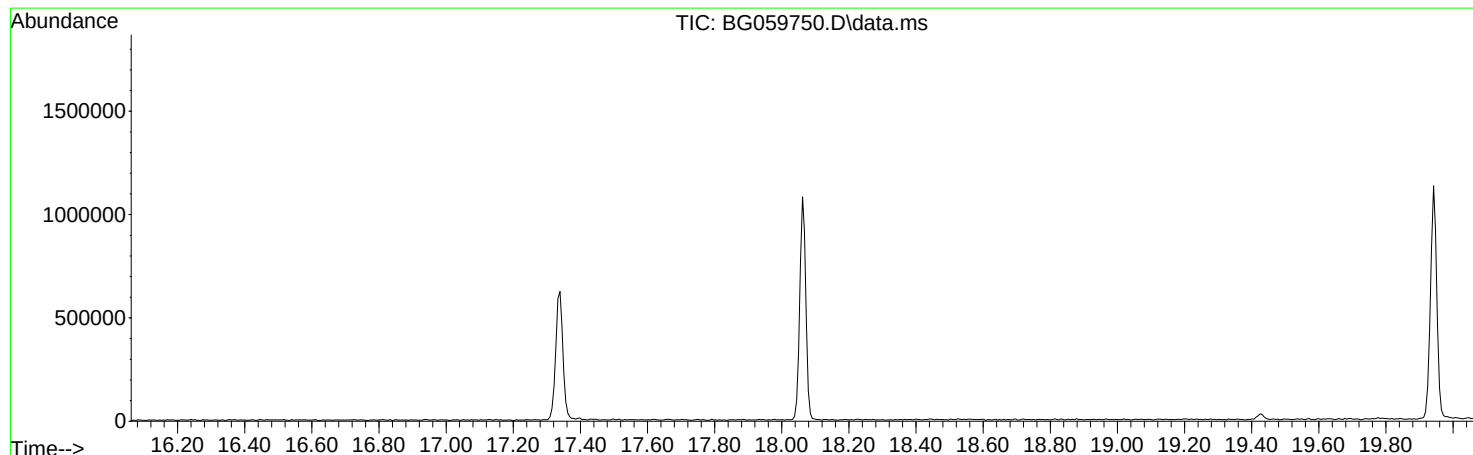




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	28960	PASS
68	69	0.00	2	1.1	421	PASS
69	198	0.00	100	59.2	38152	PASS
70	69	0.00	2	0.8	294	PASS
127	198	10	80	58.6	37768	PASS
197	198	0.00	2	0.6	363	PASS
198	198	100	100	100.0	64408	PASS
199	198	5	9	7.9	5067	PASS
275	198	10	60	33.0	21275	PASS
365	198	1	100	8.1	5247	PASS
441	198	0.01	100	15.0	9652	PASS
442	442	50	100	100.0	74981	PASS
443	442	15	24	21.2	15883	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059750.D
Acq On : 18 Nov 2023 5:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 20 07:51:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

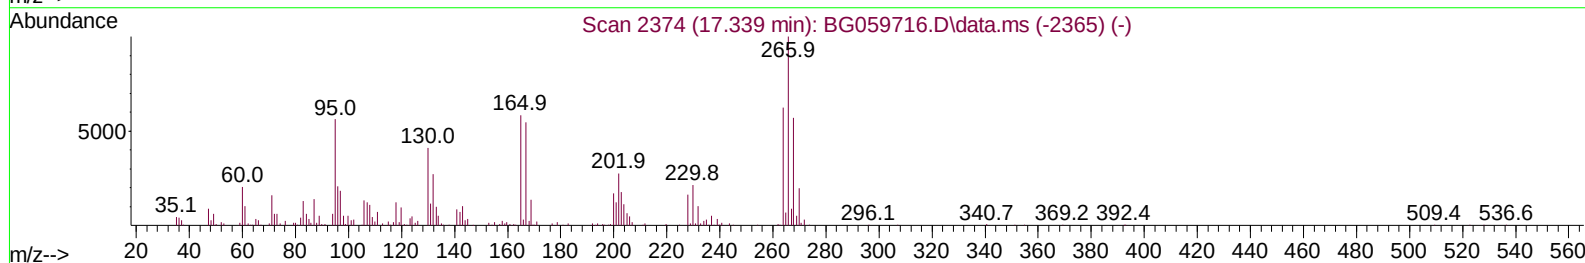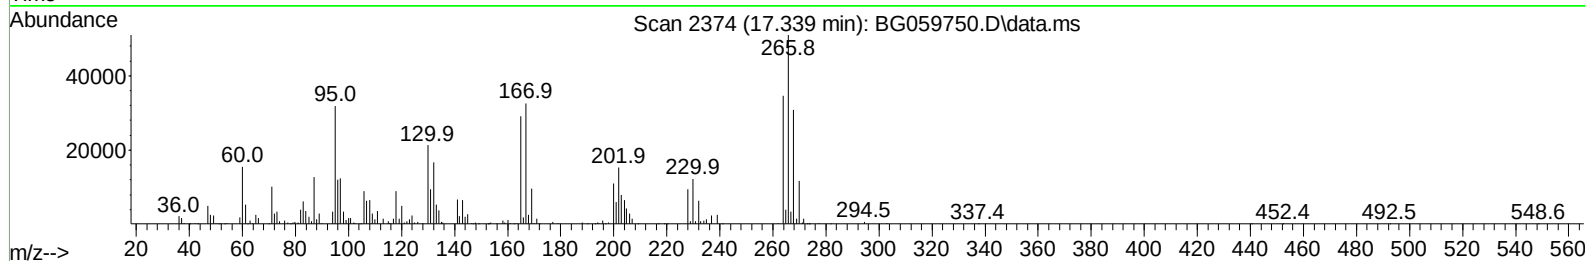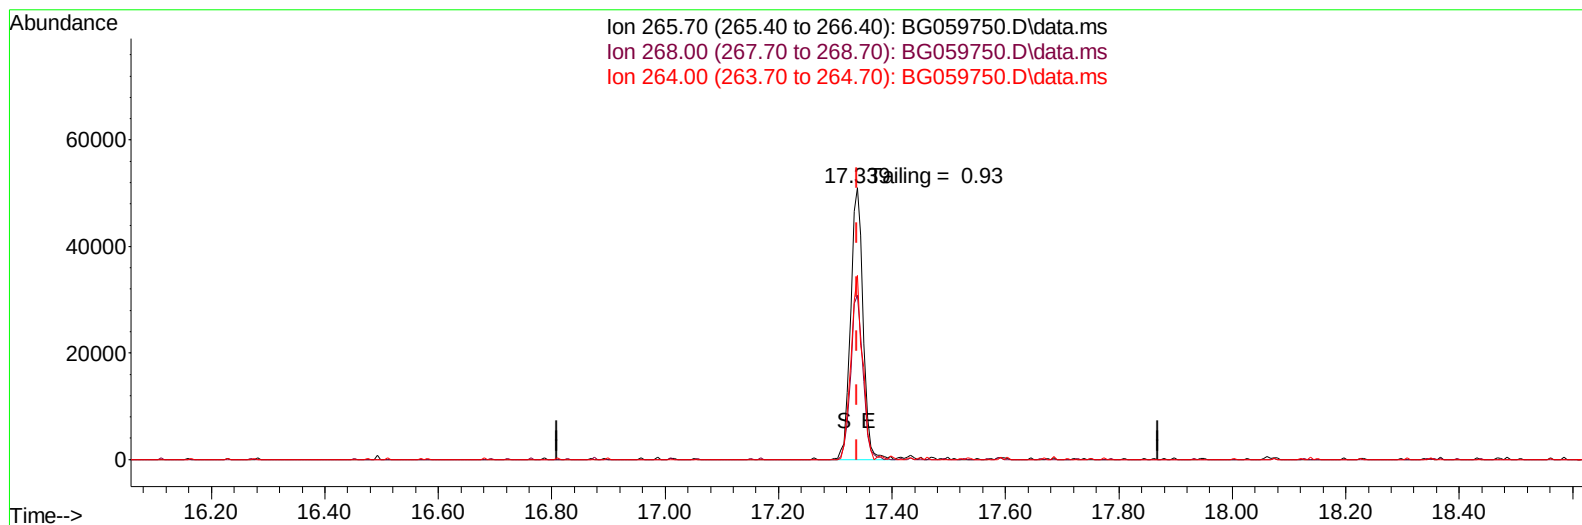

TIC: BG059750.D\data.ms

(70) Pentachlorophenol (C)

17.339min (+ 0.000) 157125.46 ng




response 78127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	60.47
264.00	62.30	67.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111723\
Data File : BG059750.D
Acq On : 18 Nov 2023 5:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 20 07:51:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

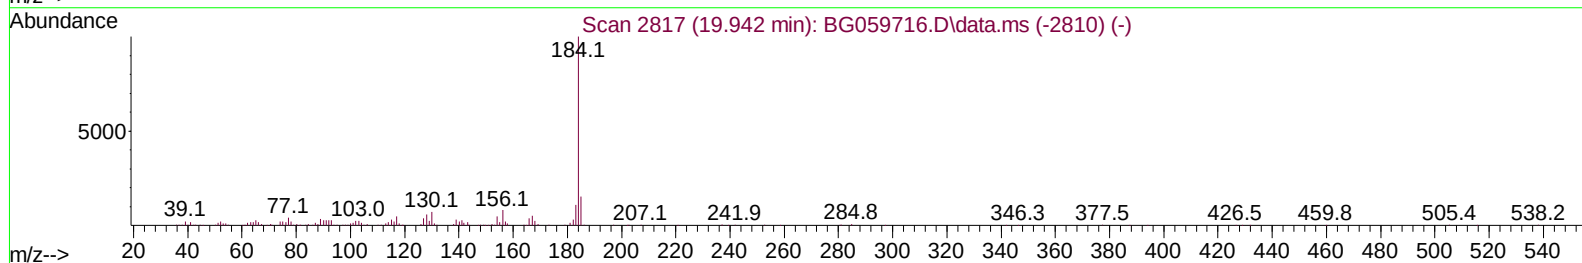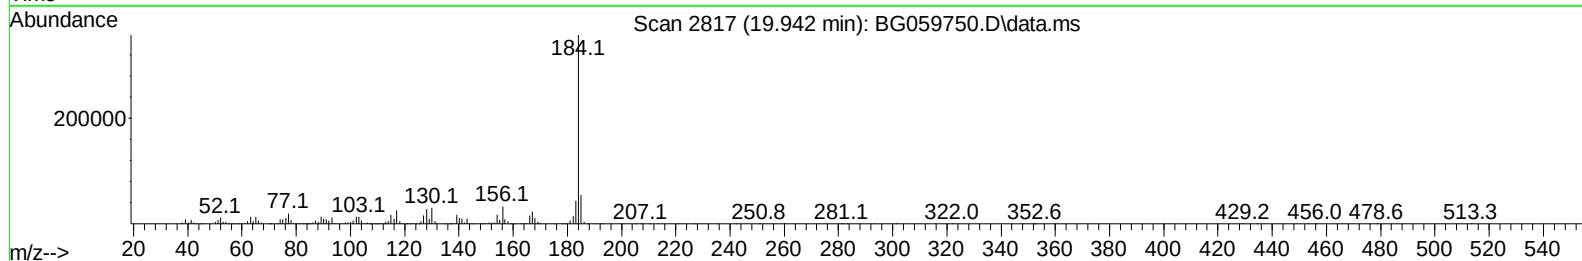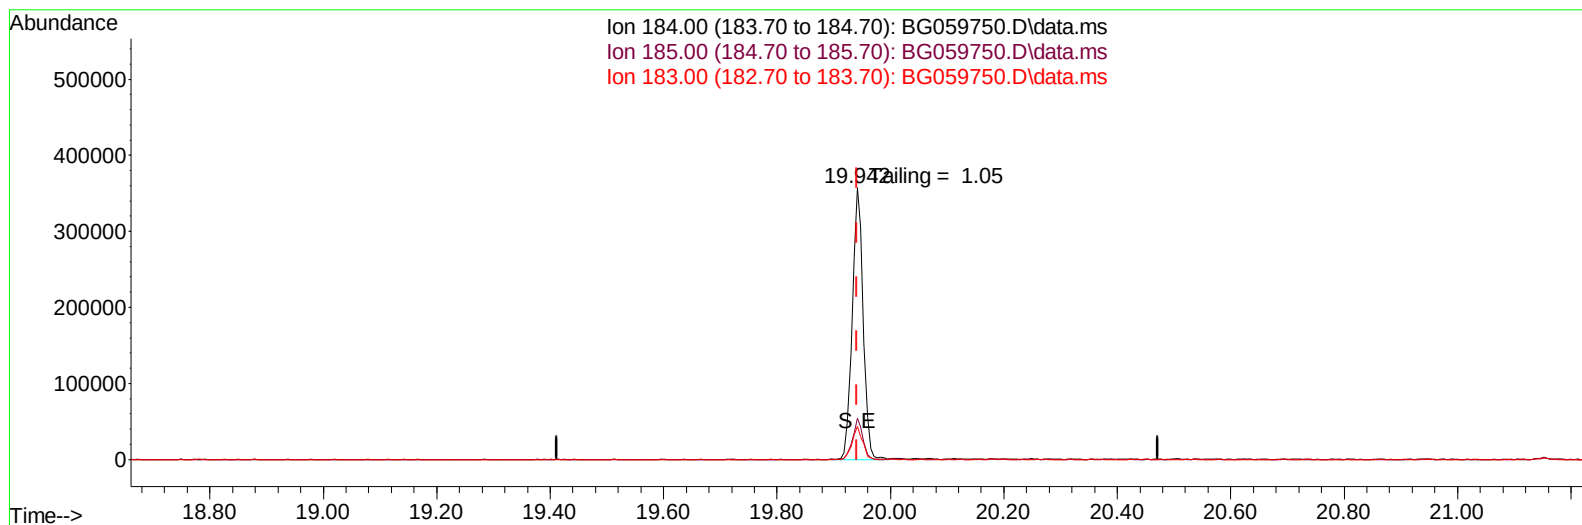

TIC: BG059750.D\data.ms

(77) Benzidine

19.942min (+ 0.000) 69956.37 ng

response 480653

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.16
183.00	11.00	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2023	BNA_G	<u>BG059750.D</u>
Compound Name	Response	Retention Time
DDT	294280	21.152
DDD	15262	20.694
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15262	309542	4.93

Instrument :
BNA_G
ClientSampleId :
DFTPP