
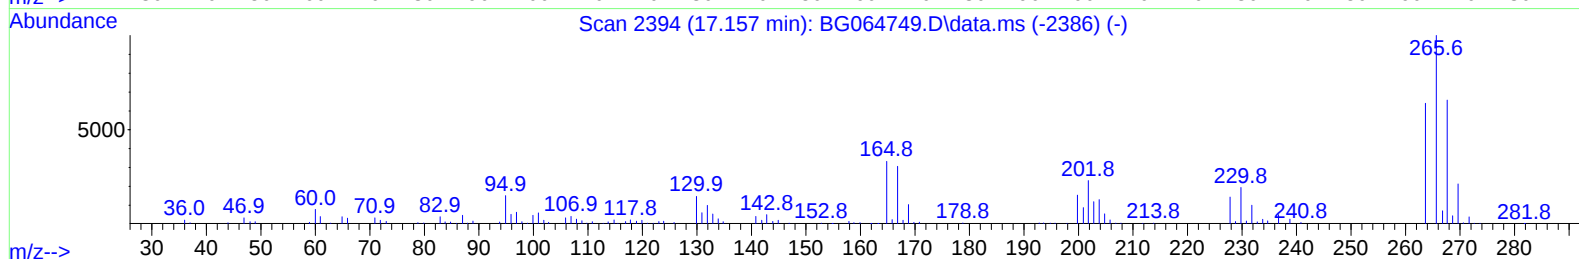
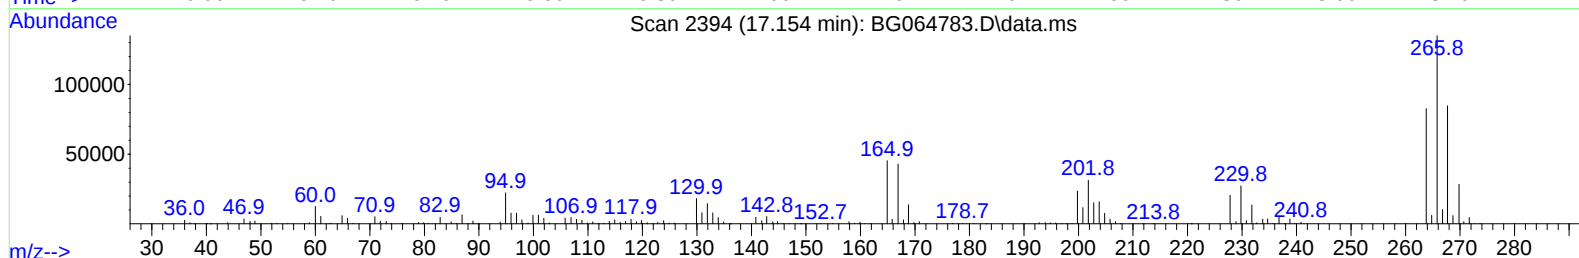


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111725\
Data File : BG064783.D
Acq On : 17 Nov 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 13:24:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

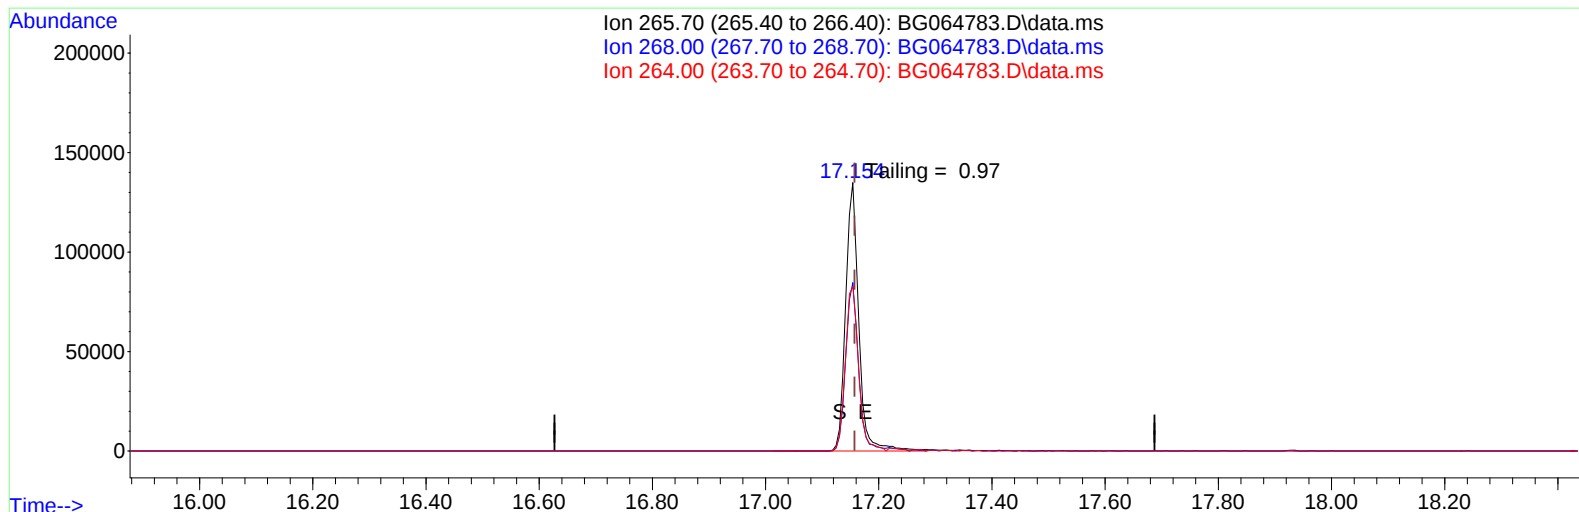

TIC: BG064783.D\data.ms

(70) Pentachlorophenol (C)




17.154min (-0.003) 35238.56 ng m

response 215947

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	62.73
264.00	64.00	61.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111725\
Data File : BG064783.D
Acq On : 17 Nov 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 13:24:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

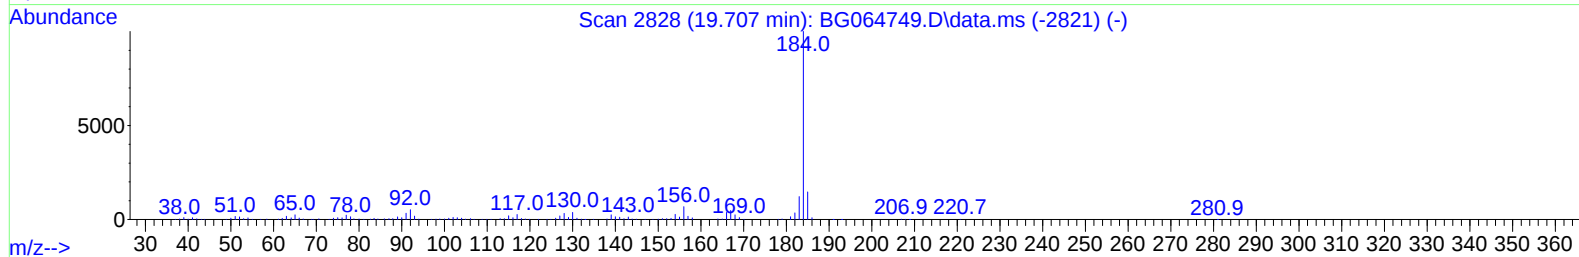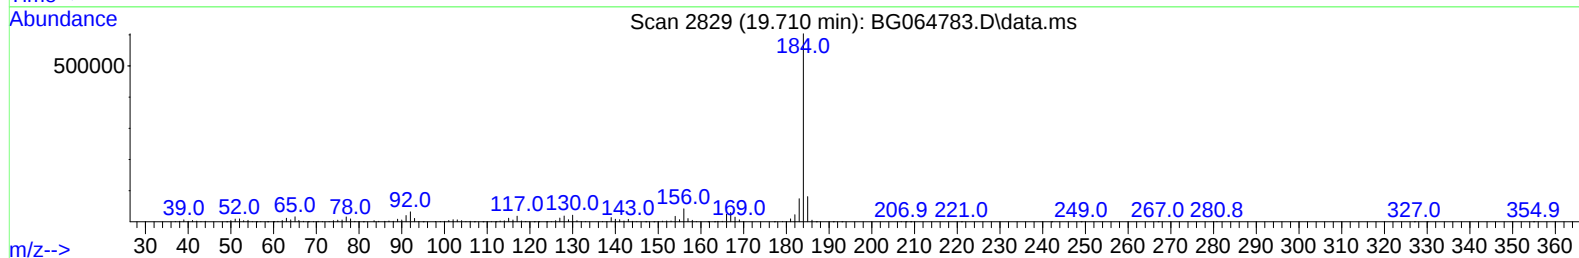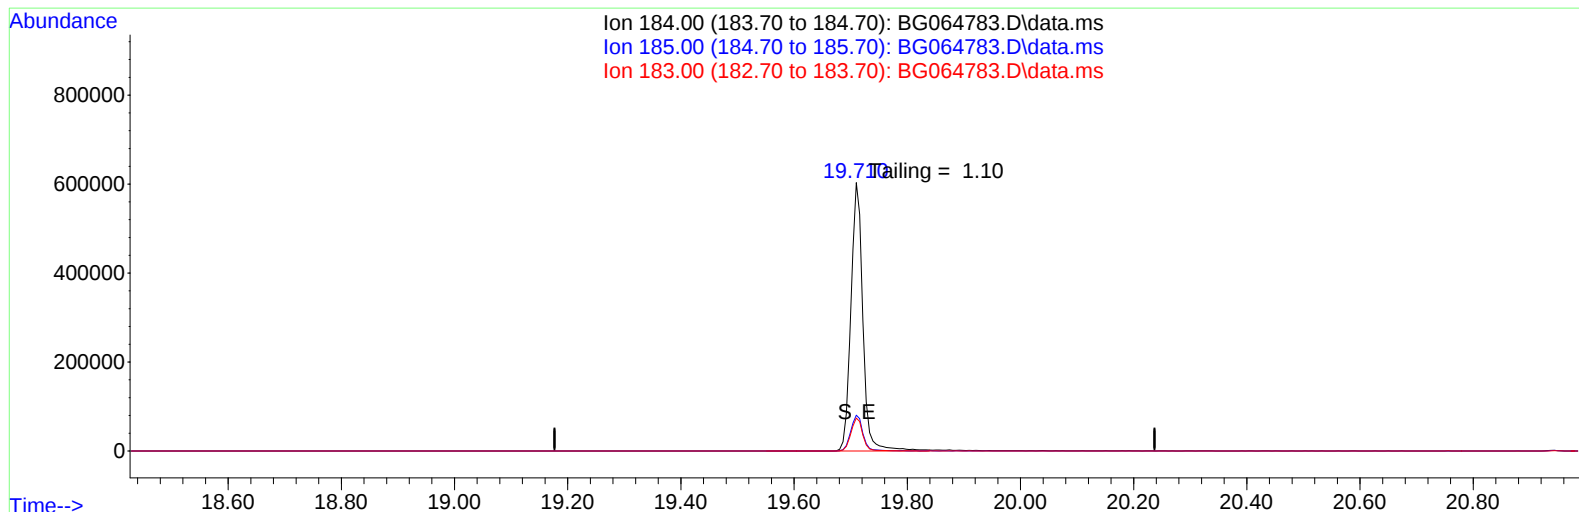

TIC: BG064783.D\data.ms

(77) Benzidine

19.710min (+ 0.003) 516560.85 ng m

response 881800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.36
183.00	12.20	12.32
0.00	0.00	0.00