

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
 Data File : BG043688.D
 Acq On : 19 Nov 2019 00:49
 Operator : JU
 Sample : K5833-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 19 01:42:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	28198	20.00	ng	-0.02
21) Naphthalene-d8	10.80	136	94282	20.00	ng	-0.02
39) Acenaphthene-d10	14.62	164	72876	20.00	ng	-0.02
64) Phenanthrene-d10	17.37	188	186728	20.00	ng	-0.02
76) Chrysene-d12	21.63	240	205617	20.00	ng	-0.02
87) Perylene-d12	24.82	264	245104	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	150675	97.92	ng	0.00
7) Phenol-d6	7.19	99	216971	98.00	ng	-0.01
23) Nitrobenzene-d5	9.15	82	122828	67.16	ng	-0.02
42) 2,4,6-Tribromophenol	16.12	330	132009	95.19	ng	-0.02
45) 2-Fluorobiphenyl	13.24	172	363705	68.96	ng	-0.02
79) Terphenyl-d14	19.98	244	760863	69.42	ng	-0.02
Target Compounds						
10) Phenol	7.21	94	8784	4.342	ng	# 55
19) n-Nitroso-di-n-propylamine	9.16	70	17907	12.517	ng	# 81
32) Benzoic acid	9.74	122	644	9.617	ng	# 1
50) Dimethylphthalate	14.08	163	38612	6.840	ng	# 98
57) 2,4-Dinitrotoluene	14.62	165	10167	5.801	ng	# 28
67) 4-Bromophenyl-phenylether	16.12	248	8112	3.228	ng	# 1
77) Benzidine	19.98	184	11496	2.778	ng	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
Data File : BG043688.D
Acq On : 19 Nov 2019 00:49
Operator : JU
Sample : K5833-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 19 01:42:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

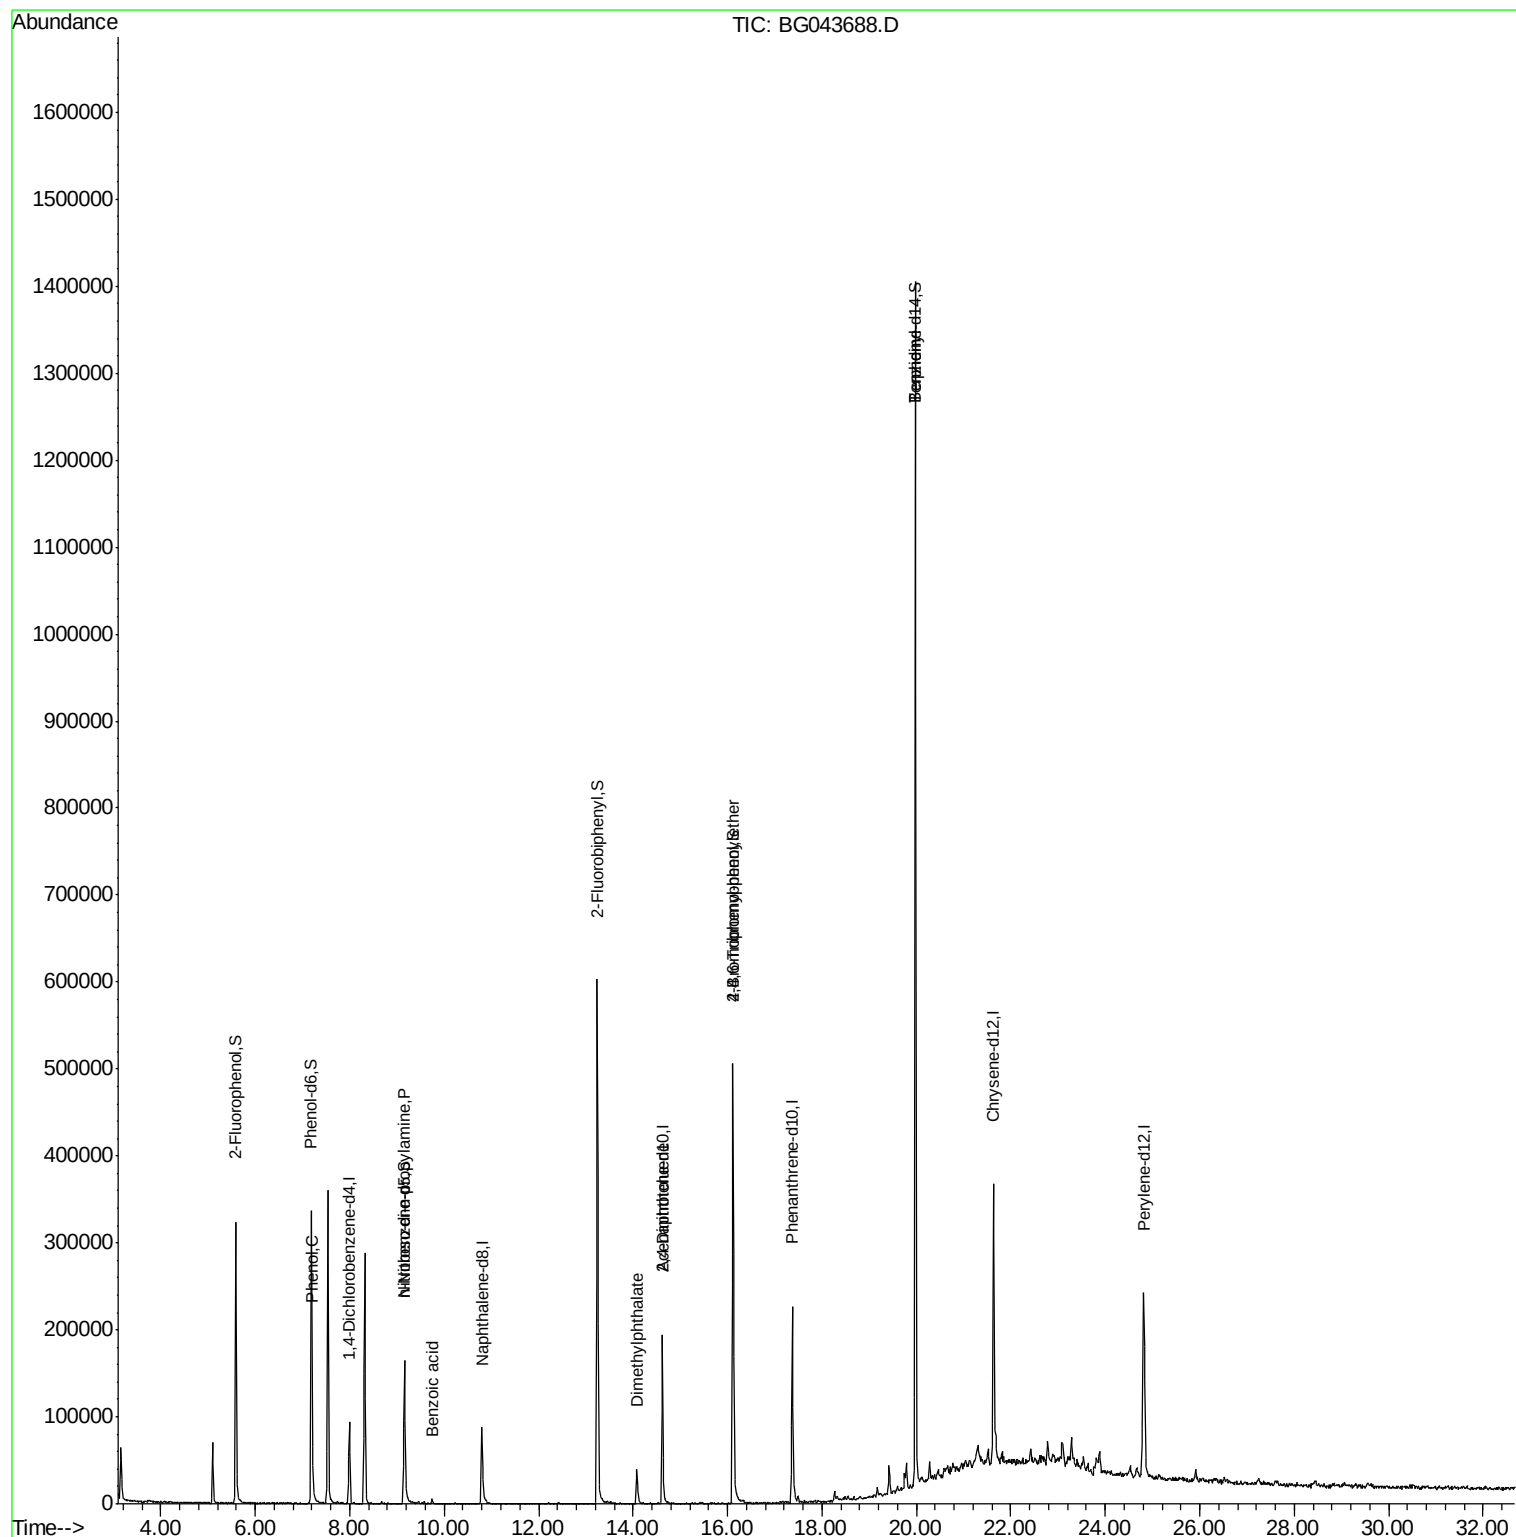

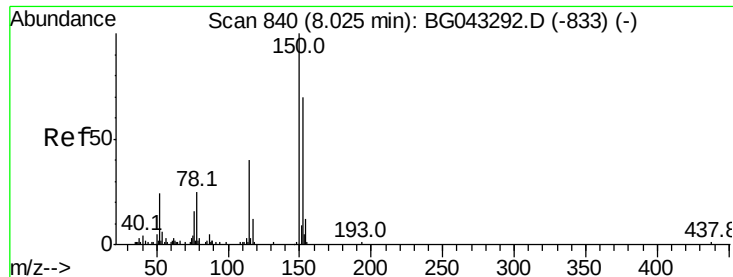


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 834
Delta R.T. -0.02 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 28198
Ion Ratio Lower Upper
152 100
150 155.5 129.4 194.0
115 67.4 48.8 73.2

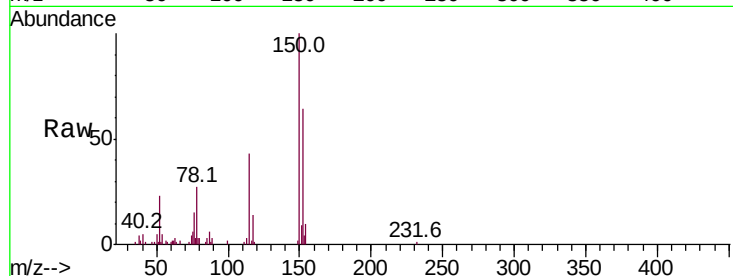


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

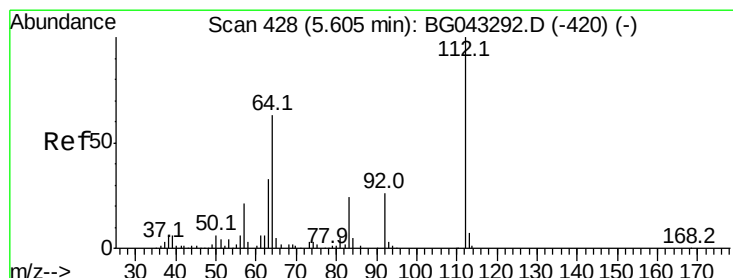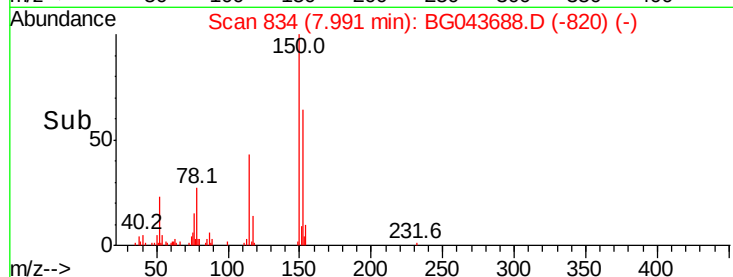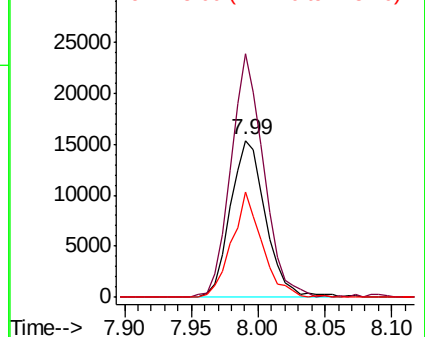



#5




2-Fluorophenol
Concen: 97.916 ng
RT: 5.59 min Scan# 425
Delta R.T. -0.01 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Tgt Ion:112 Resp: 150675
Ion Ratio Lower Upper
112 100
64 60.3 50.0 75.0
63 36.4 26.6 40.0

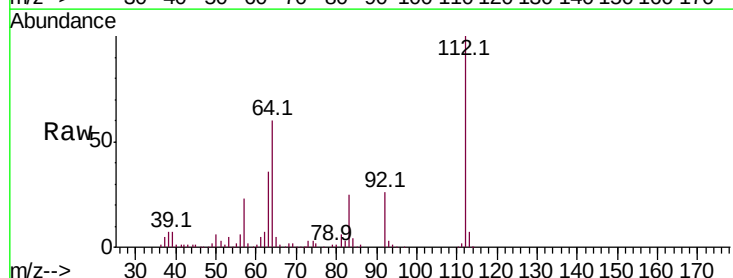

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

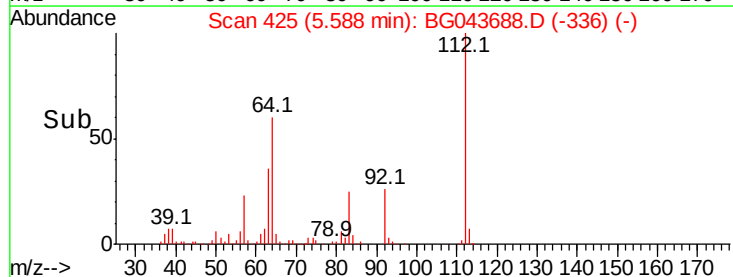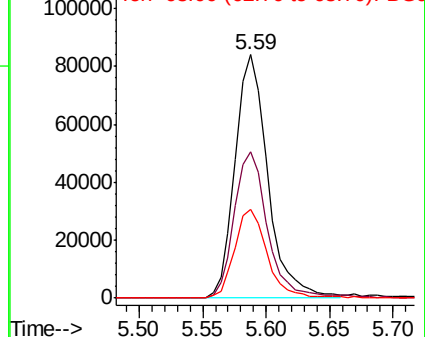

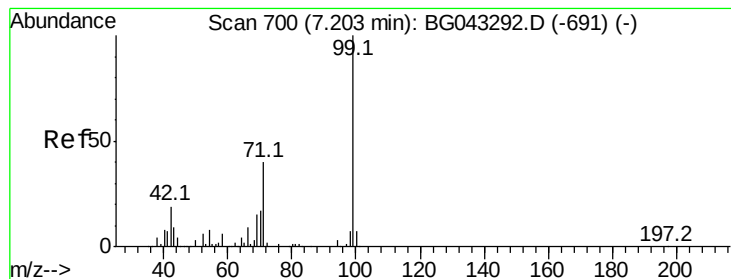

#7

Phenol-d6

Concen: 98.000 ng

RT: 7.19 min Scan# 697

Delta R.T. -0.01 min

Lab File: BG043688.D

Acq: 19 Nov 2019 00:49

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 99 Resp: 216971

Ion Ratio Lower Upper

99 100

42 20.2 14.6 21.8

71 40.6 32.5 48.7

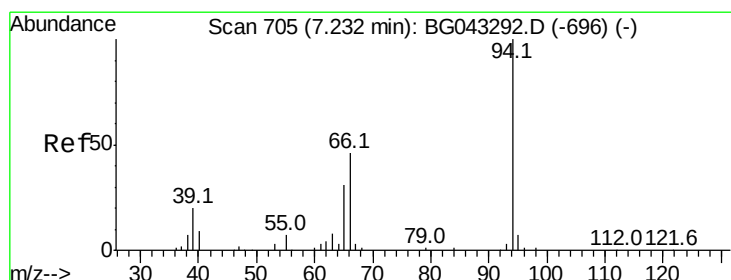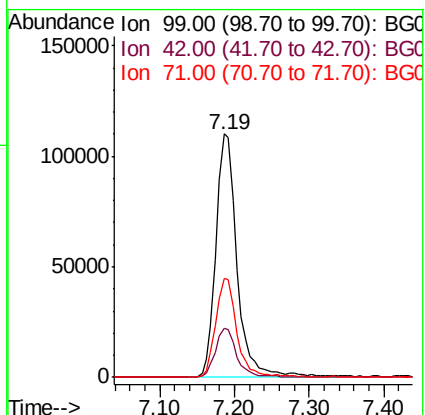

#10

Phenol

Concen: 4.342 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.01 min

Lab File: BG043688.D

Acq: 19 Nov 2019 00:49


Tgt Ion: 94 Resp: 8784


Ion Ratio Lower Upper

94 100

65 51.1 12.6 52.6

66 87.2 30.7 70.7#




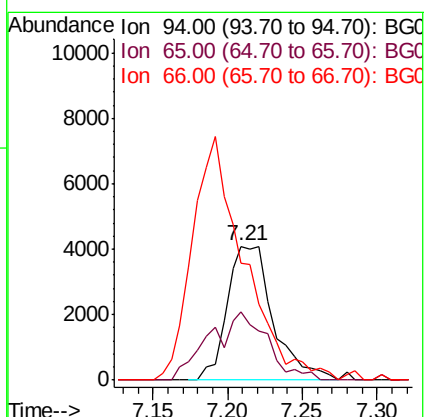


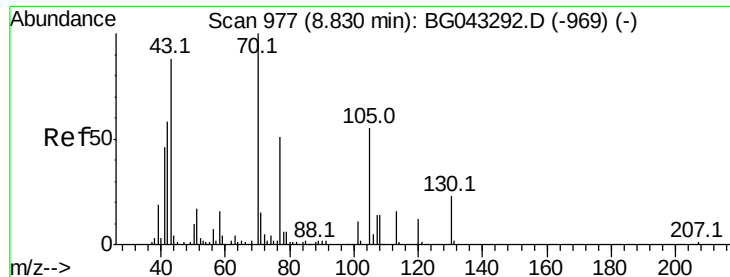

#19
n-Nitroso-di-n-propylamine
Concen: 12.517 ng
RT: 9.16 min Scan# 1033
Delta R.T. 0.35 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49




Instrument :
BNA_G
ClientSampleId :


Tot Ion: 70 Resp: 17907
Ion Ratio Lower Upper
70 100
42 46.7 41.4 62.2
101 0.0 7.9 11.9#
130 2.6 19.0 28.4#

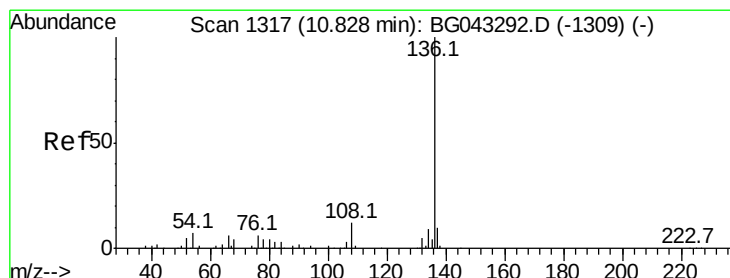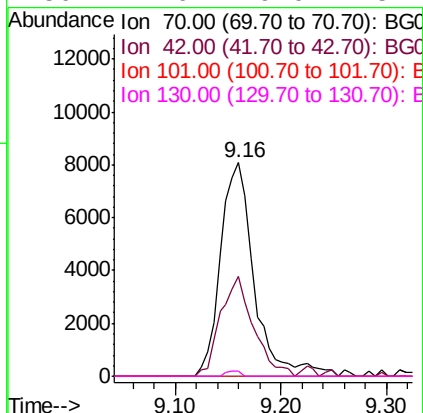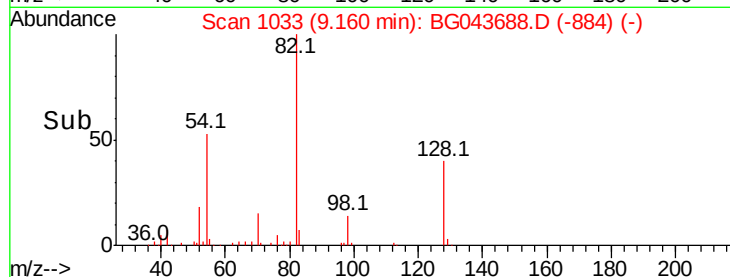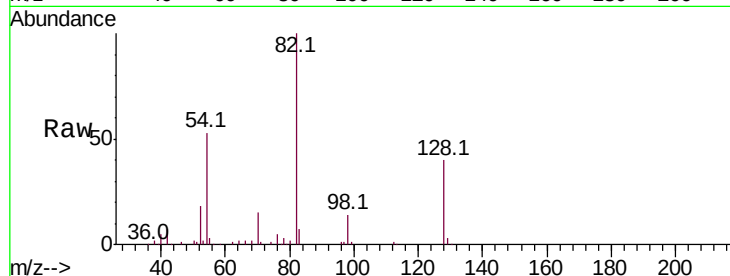

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.80 min Scan# 1312
Delta R.T. -0.02 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Tgt Ion:136 Resp: 94282
Ion Ratio Lower Upper
136 100
137 12.6 8.7 13.1
54 9.2 5.4 8.2#
68 4.2 3.0 4.4

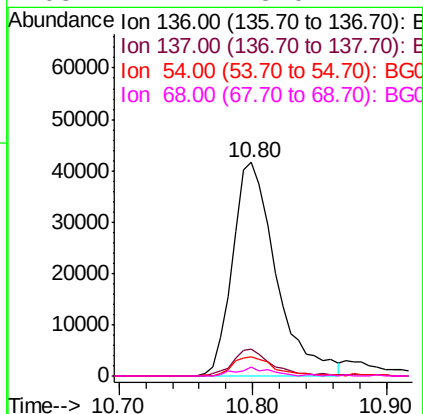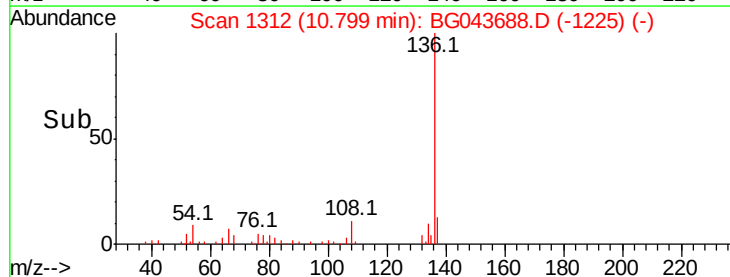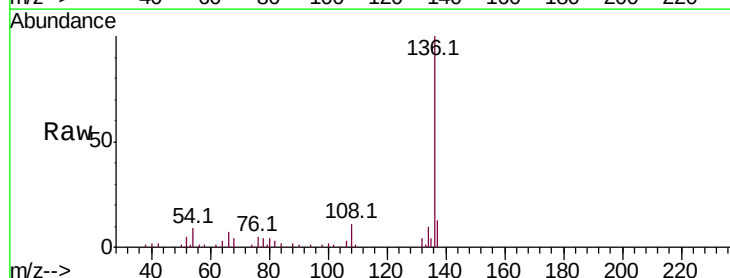







#23
Nitrobenzene-d5
Concen: 67.164 ng
RT: 9.15 min Scan# 1032
Delta R.T. -0.02 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Instrument :
BNA_G
ClientSampleId :

Tot Ion: 82 Resp: 122828
Ion Ratio Lower Upper
82 100
128 44.2 35.0 52.6
54 58.0 40.2 60.2




Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC


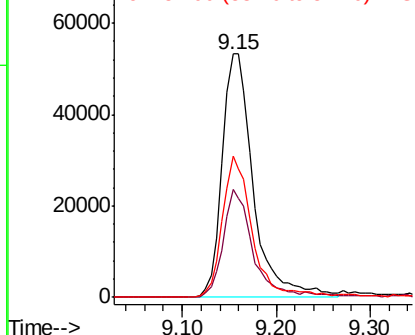



#32
Benzoic acid
Concen: 9.617 ng
RT: 9.74 min Scan# 1132
Delta R.T. -0.42 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Tgt Ion: 122 Resp: 644
Ion Ratio Lower Upper
122 100
105 0.0 103.3 143.3#
77 0.0 84.9 124.9#



Abundance Ion 122.00 (121.70 to 122.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 77.00 (76.70 to 77.70): BGC




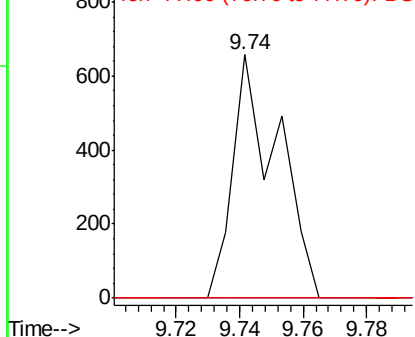


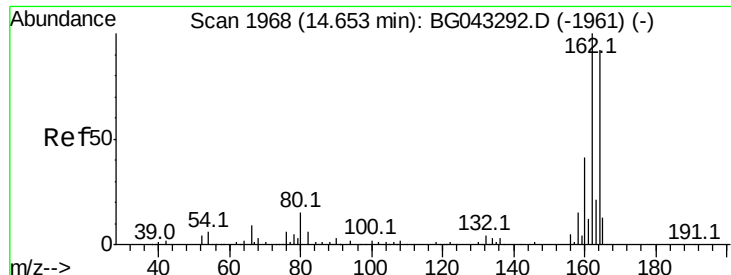

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.62 min Scan# 1963
Delta R.T. -0.02 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49




Instrument :
BNA_G
ClientSampleId :


Tot Ion:164 Resp: 72876
Ion Ratio Lower Upper
164 100
162 106.5 83.5 125.3
160 46.0 36.5 54.7

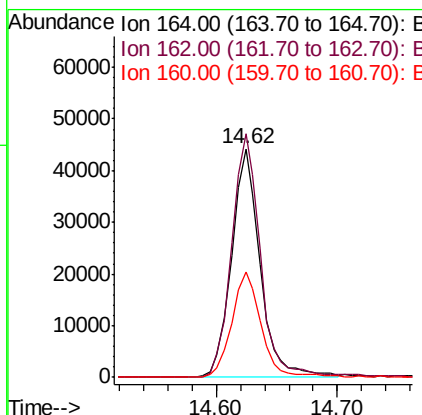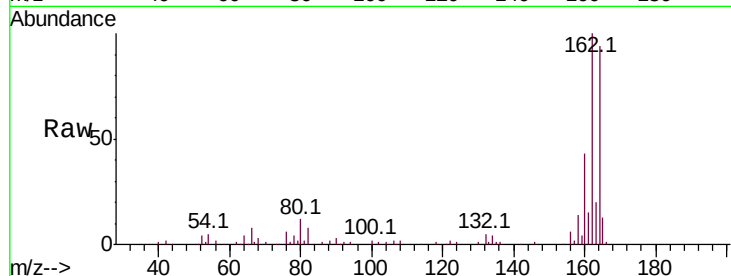

#42
2,4,6-Tribromophenol
Concen: 95.187 ng
RT: 16.12 min Scan# 2217
Delta R.T. -0.02 min
Lab File: BG043688.D
Acq: 19 Nov 2019 00:49

Tgt Ion:330 Resp: 132009
Ion Ratio Lower Upper
330 100
332 94.5 77.4 116.0
141 29.0 22.8 34.2

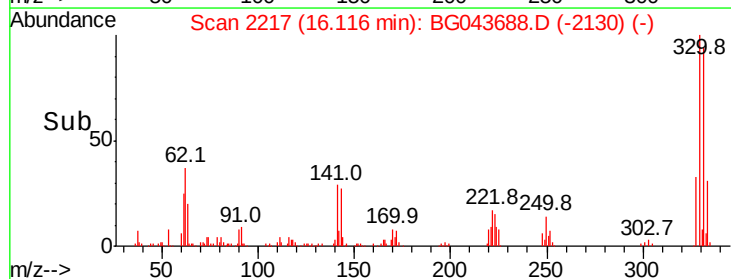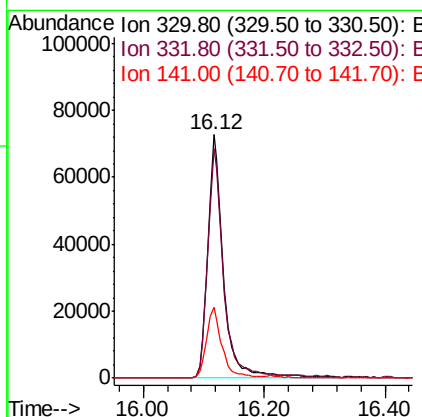







#45
 2-Fluorobiphenyl
 Concen: 68.962 ng
 RT: 13.24 min Scan# 1728
 Delta R.T. -0.02 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:172 Resp: 363705




Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.9	43.3
170	23.2	18.5	27.7

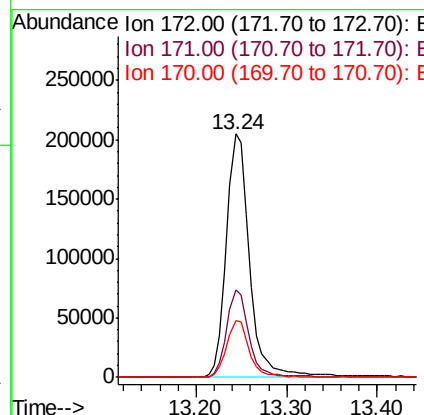


#50
 Dimethylphthalate
 Concen: 6.840 ng
 RT: 14.08 min Scan# 1870
 Delta R.T. -0.02 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49

Tgt Ion:163 Resp: 38612

Ion	Ratio	Lower	Upper
163	100		
194	2.8	3.8	5.6#
164	10.8	8.9	13.3

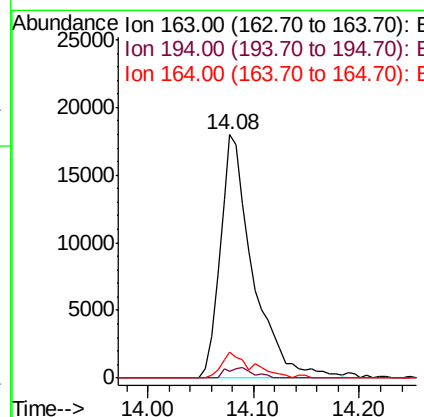




#57
 2,4-Dinitrotoluene
 Concen: 5.801 ng
 RT: 14.62 min Scan# 1963
 Delta R.T. -0.38 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	3.4	33.2	49.8#
89	0.0	52.2	78.4#
182	0.0	2.0	3.0#



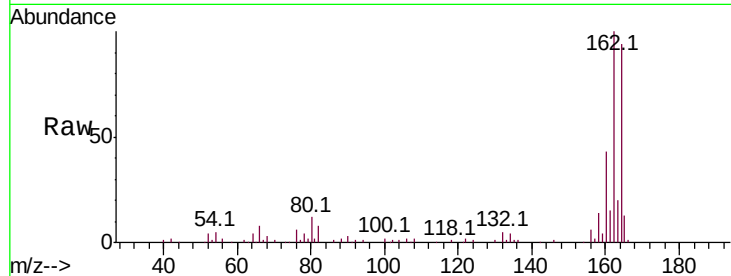


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

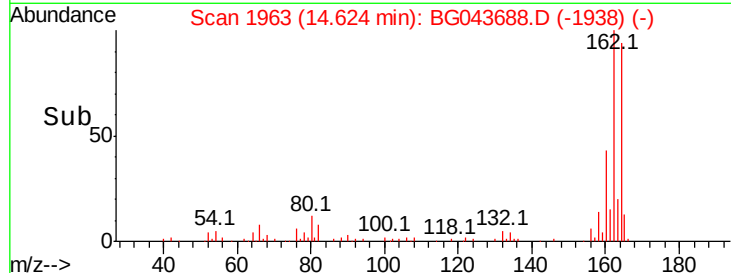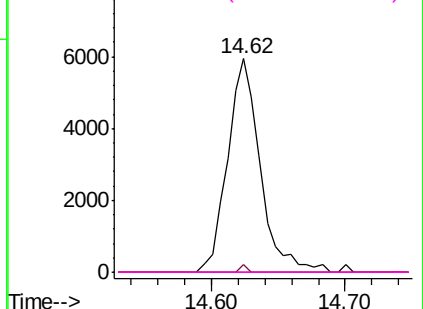

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.37 min Scan# 2430
 Delta R.T. -0.02 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49



Tgt Ion	Ratio	Lower	Upper
188	100		
94	5.9	4.2	6.4
80	6.2	4.5	6.7

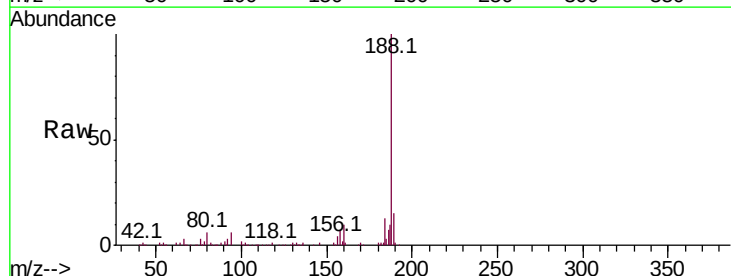


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

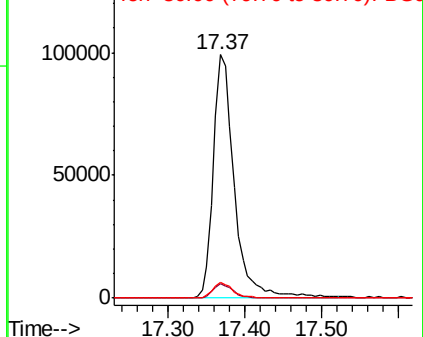


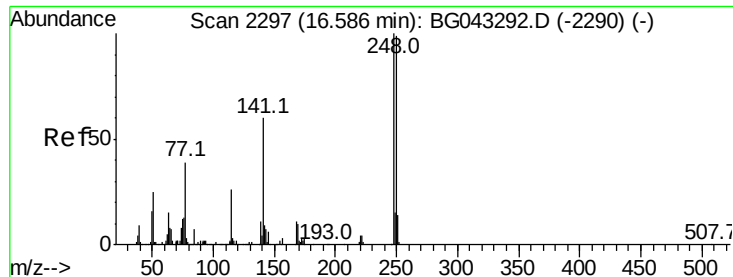




#67
 4-Bromophenyl-phenylether
 Concen: 3.228 ng
 RT: 16.12 min Scan# 2217
 Delta R.T. -0.46 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:248 Resp: 8112
 Ion Ratio Lower Upper
 248 100
 250 227.1 77.0 115.4#
 141 468.9 47.5 71.3#

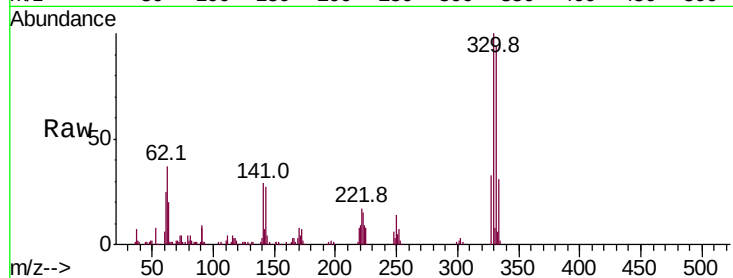


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

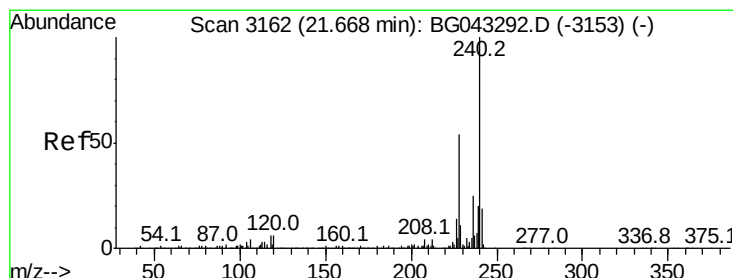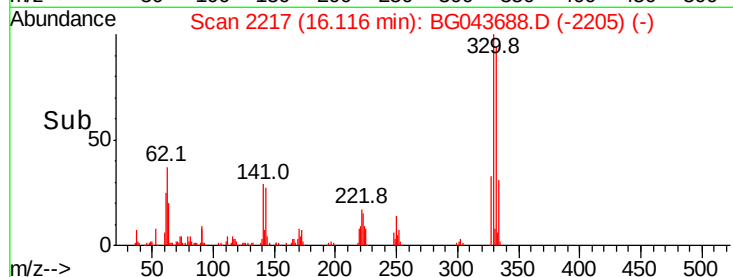
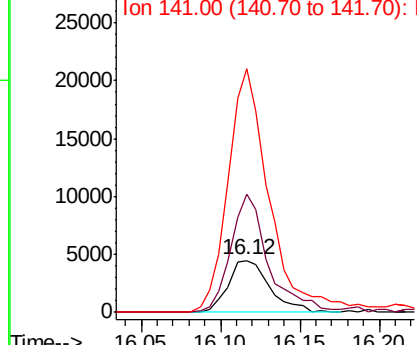



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.63 min Scan# 3156
 Delta R.T. -0.02 min
 Lab File: BG043688.D
 Acq: 19 Nov 2019 00:49

Tgt Ion:240 Resp: 205617
 Ion Ratio Lower Upper
 240 100
 120 5.9 4.6 6.8
 236 25.2 19.8 29.8

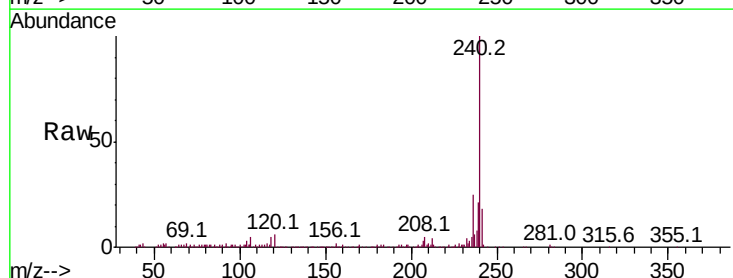

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

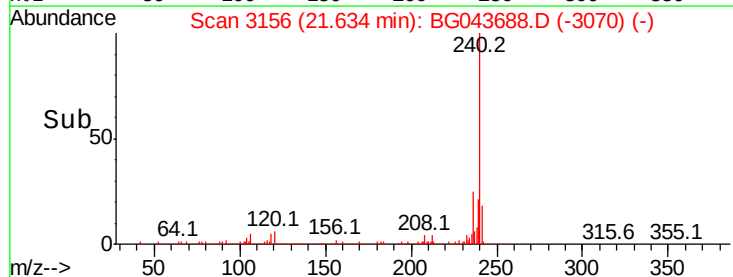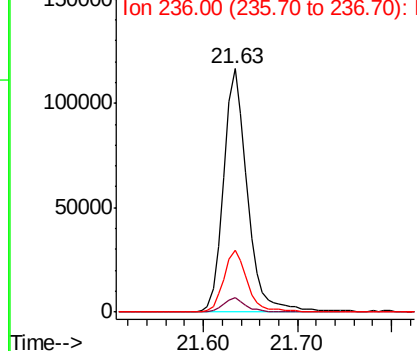

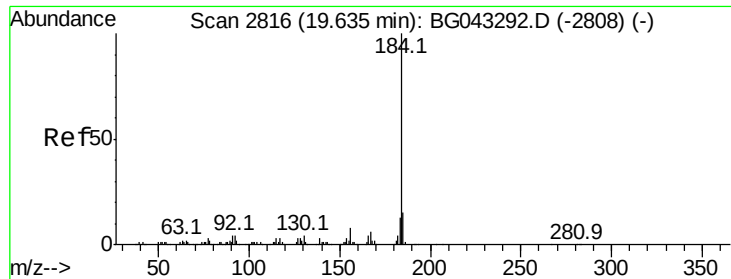

#77

Benzidine

Concen: 2.778 ng

RT: 19.98 min Scan# 2875

Delta R.T. 0.36 min

Lab File: BG043688.D

Acq: 19 Nov 2019 00:49

Instrument :

BNA_G

ClientSampled :


Tot Ion:184 Resp: 11496

Ion Ratio Lower Upper

184 100

185 27.4 11.0 16.4#




183 7.7 10.0 15.0#

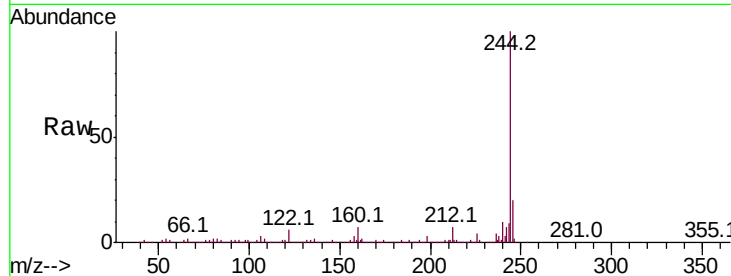

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

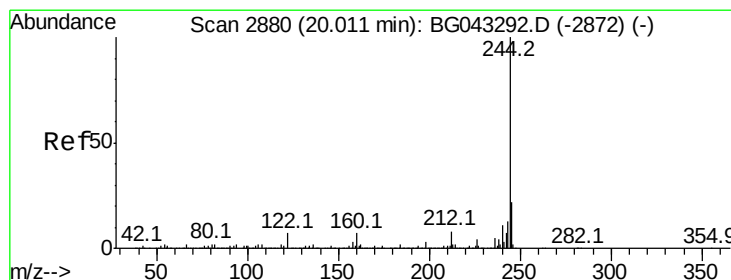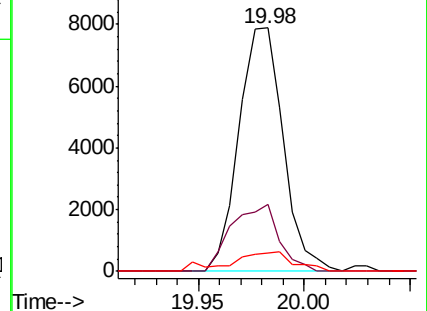

#79

Terphenyl-d14

Concen: 69.421 ng

RT: 19.98 min Scan# 2875

Delta R.T. -0.02 min

Lab File: BG043688.D

Acq: 19 Nov 2019 00:49


Tgt Ion:244 Resp: 760863

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.6



122 6.0 5.4 8.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

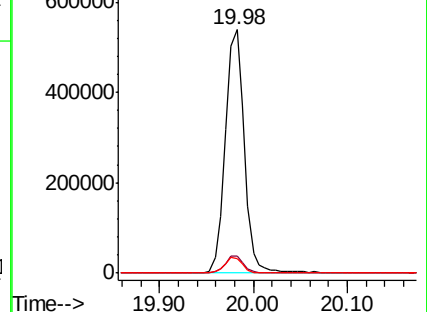

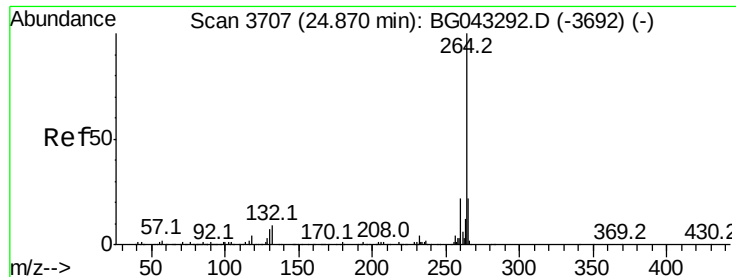

#87

Pervlene-d12

Concen: 20.000 ng

RT: 24.82 min Scan# 3698

Delta R.T. -0.03 min

Lab File: BG043688.D

Acq: 19 Nov 2019 00:49

Instrument :

BNA_G

ClientSampleId :


Tot Ion:264 Resp: 245104

Ion Ratio Lower Upper

264 100

260 23.2 17.5 26.3

265 19.6 17.4 26.0

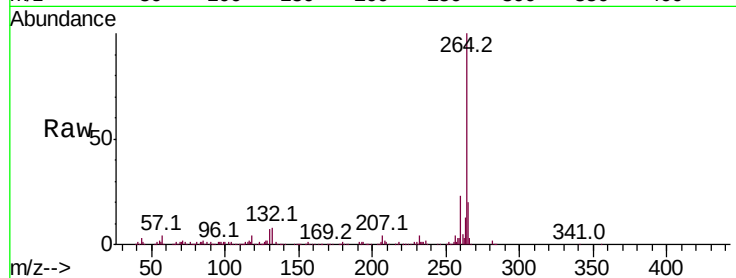

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

