
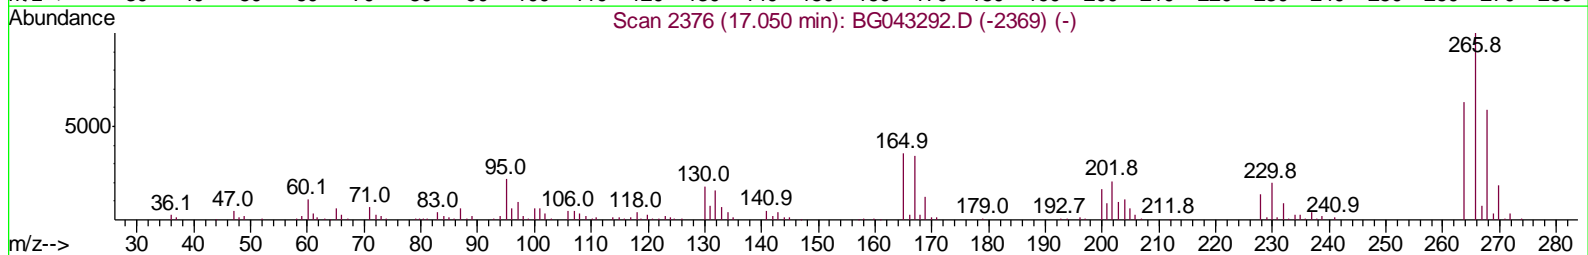
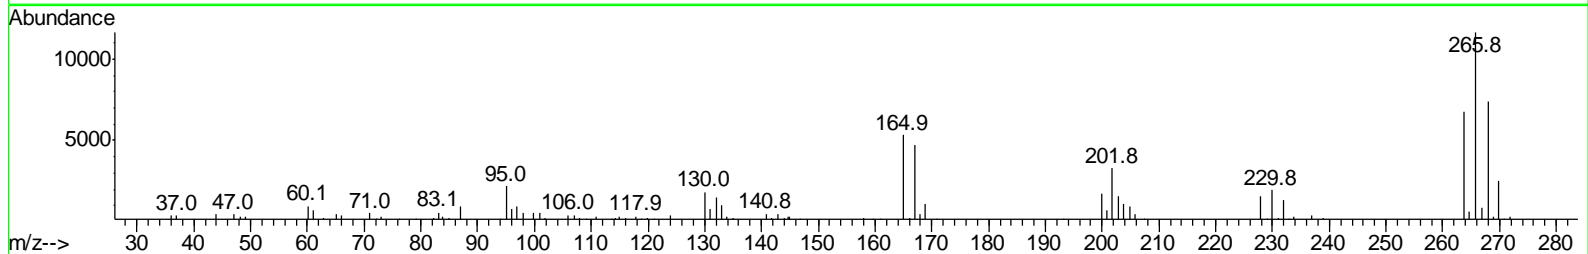


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
 Data File : BG043672.D
 Acq On : 18 Nov 2019 14:20
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 03:06:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

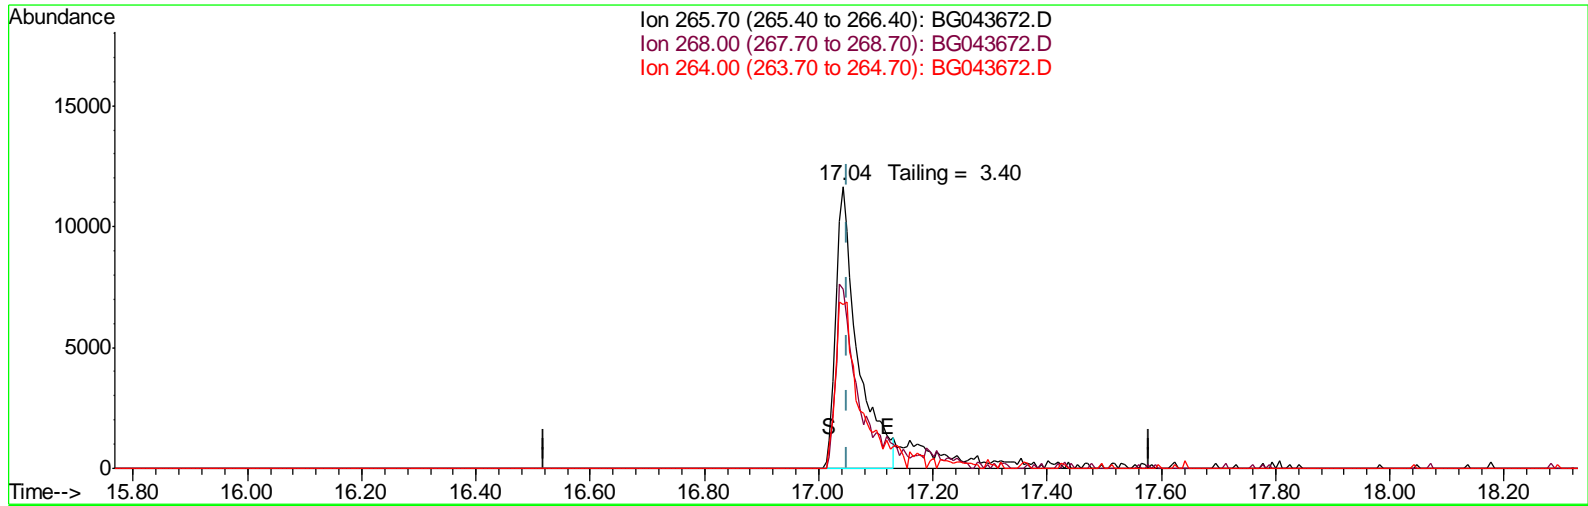




TIC: BG043672.D

(70) Pentachlorophenol (C)
 17.042min (-0.007) 34909.04ng m
 response 31207

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	63.72
264.00	61.10	58.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
 Data File : BG043672.D
 Acq On : 18 Nov 2019 14:20
 Operator : JU
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 03:06:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

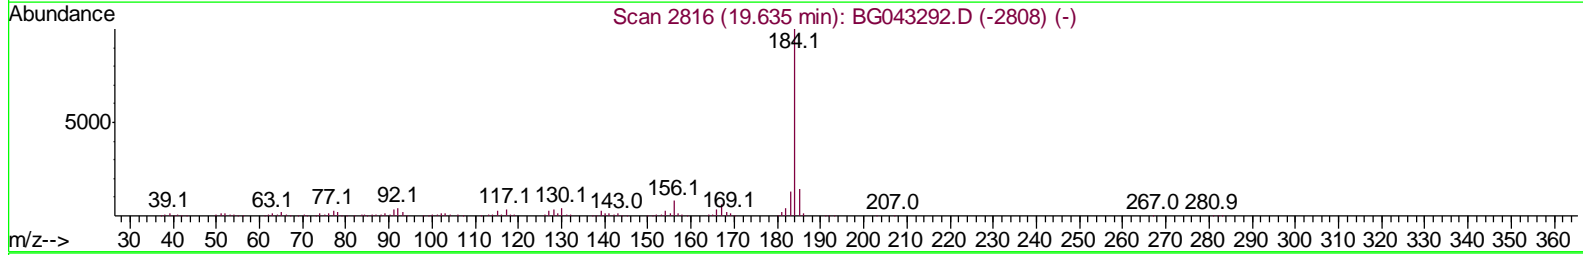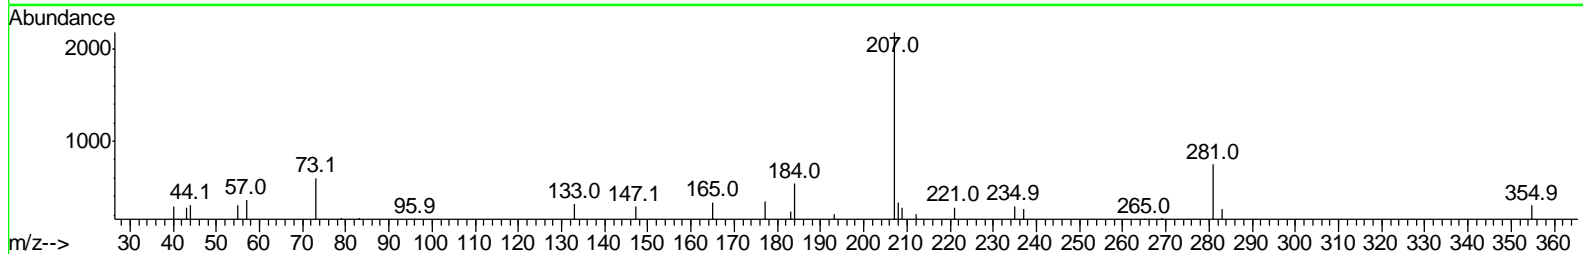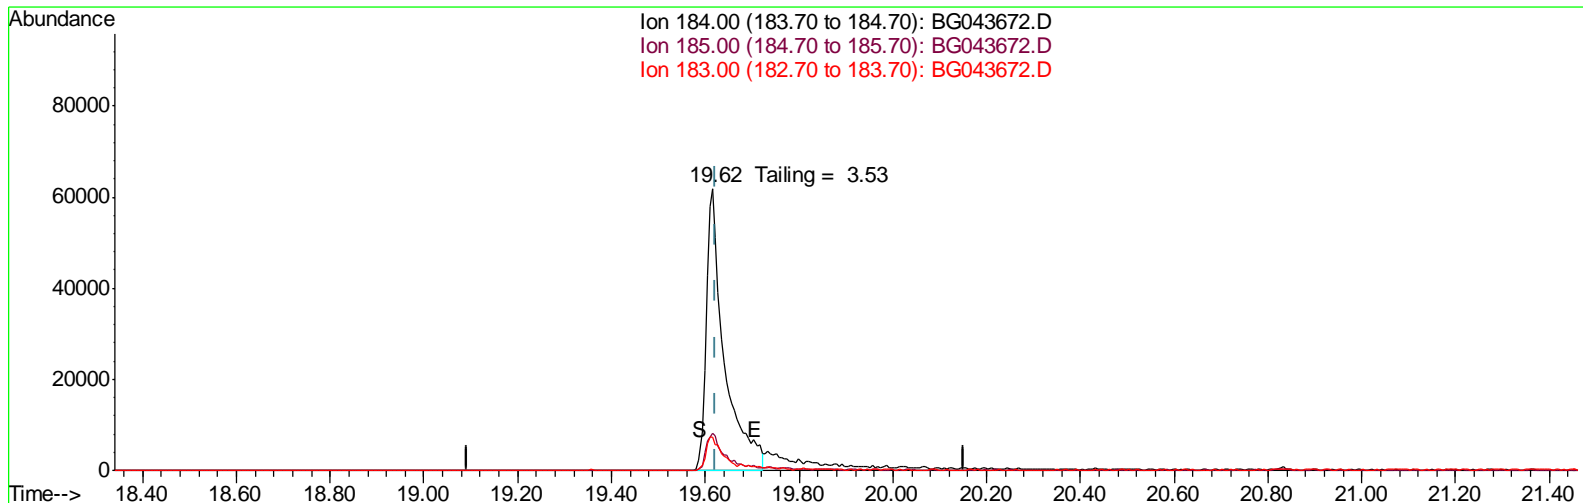

TIC: BG043672.D

(77) Benzidine

20.433min (+0.809) 709.72ng

response 857

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	0.00#
183.00	12.50	42.67#
0.00	0.00	0.00