

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
 Data File : BG043685.D
 Acq On : 18 Nov 2019 22:51
 Operator : JU
 Sample : K5782-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-2A-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.190	9	17	25	rVB	395265	780218	27.85%	6.181%
2	3.472	60	65	71	rVB	45154	60980	2.18%	0.483%
3	3.889	132	136	146	rBV	48923	70772	2.53%	0.561%
4	4.494	234	239	251	rVB	363362	543174	19.39%	4.303%
5	4.617	254	260	266	rBV4	21511	36054	1.29%	0.286%
6	5.099	339	342	349	rVB	59026	89603	3.20%	0.710%
7	5.587	418	425	439	rBV	481248	827469	29.54%	6.556%
8	7.132	683	688	691	rBV2	18462	29671	1.06%	0.235%
9	7.191	691	698	714	rVB	464947	846062	30.20%	6.703%
10	7.538	749	757	766	rBV	510843	915370	32.68%	7.252%
11	7.990	827	834	843	rBV	90228	158360	5.65%	1.255%
12	8.319	879	890	902	rBV	392959	714178	25.49%	5.658%
13	9.159	1025	1033	1047	rBV	249357	531709	18.98%	4.213%
14	10.798	1304	1312	1330	rBV	80630	194338	6.94%	1.540%
15	13.243	1721	1728	1743	rBV	763711	1322860	47.22%	10.481%
16	14.623	1955	1963	1976	rBV	154820	285240	10.18%	2.260%
17	16.116	2210	2217	2243	rBV	642874	1212065	43.27%	9.603%
18	17.373	2422	2431	2446	rBV	191278	378471	13.51%	2.999%
19	19.982	2868	2875	2895	rBV	1963796	2801346	100.00%	22.194%
20	21.639	3150	3157	3169	rBV2	252670	513936	18.35%	4.072%
21	24.817	3688	3698	3712	rBV4	86225	310014	11.07%	2.456%


Sum of corrected areas: 12621890

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111819\
Data File : BG043685.D
Acq On : 18 Nov 2019 22:51
Operator : JU
Sample : K5782-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2A-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

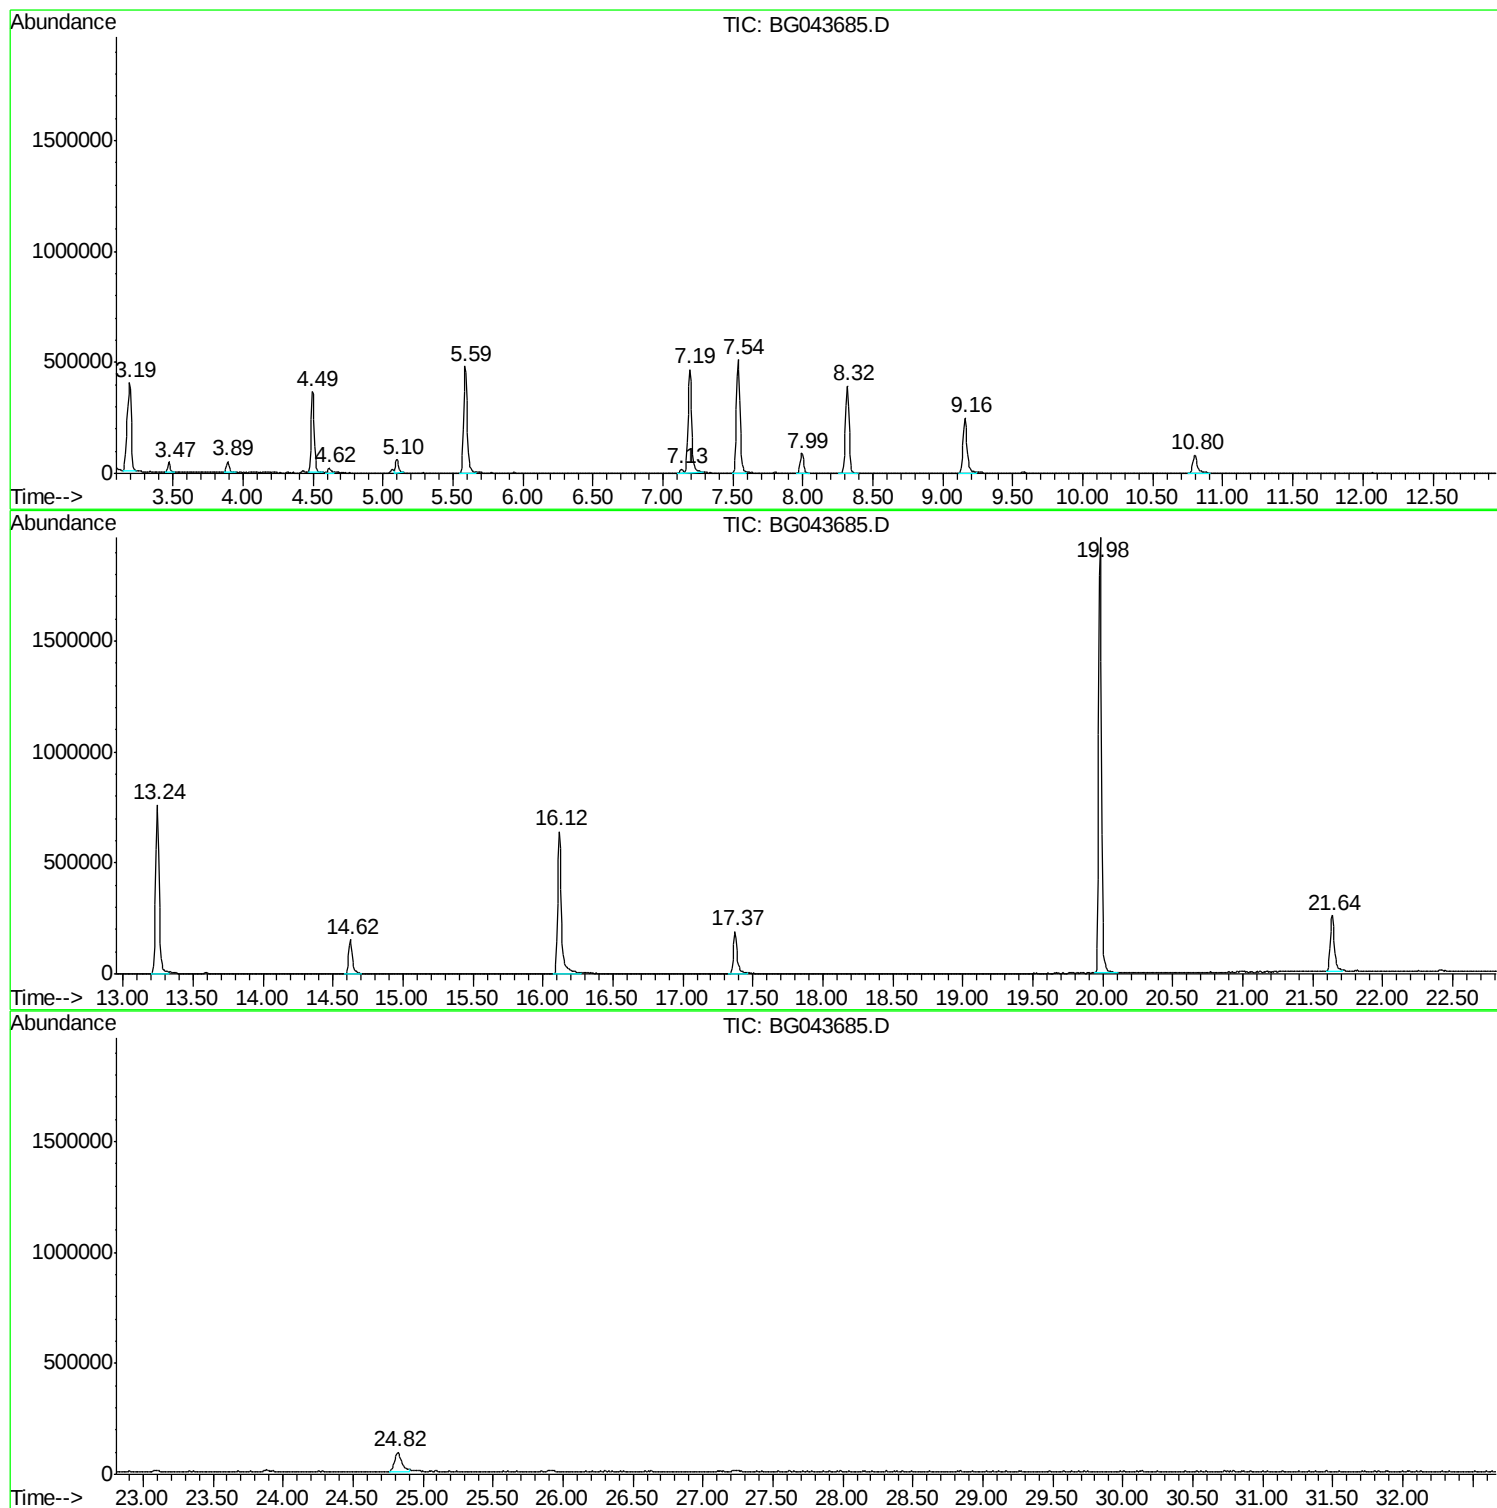

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111819\
Data_File : BG043685.D
Acq_On : 18 Nov 2019 22:511
Operator : JUJ
Sample : K5782-088
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
TP-2A-COMP

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
