


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111819\
 Data File : BG043672.D
 Acq On : 18 Nov 2019 14:20
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 19 15:23:15 2019

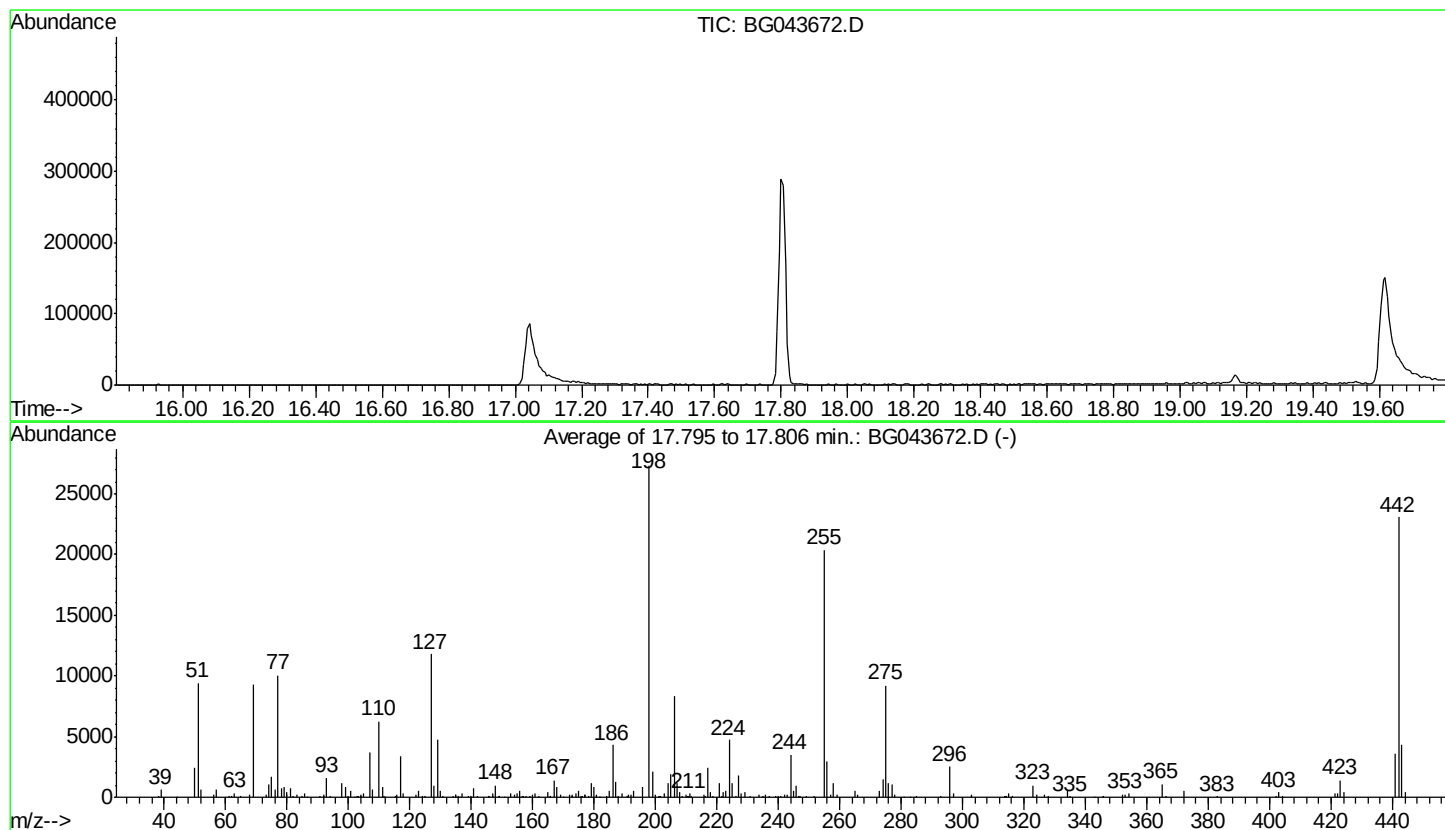

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	9400	PASS
68	69	0.00	2	1.8	168	PASS
69	198	0.00	100	33.9	9268	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	11790	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27330	PASS
199	198	5	9	7.8	2139	PASS
275	198	10	60	33.6	9191	PASS
365	198	1	100	4.0	1099	PASS
441	198	0.01	100	13.3	3642	PASS
442	198	50	100	84.4	23064	PASS
443	442	15	24	18.8	4333	PASS