
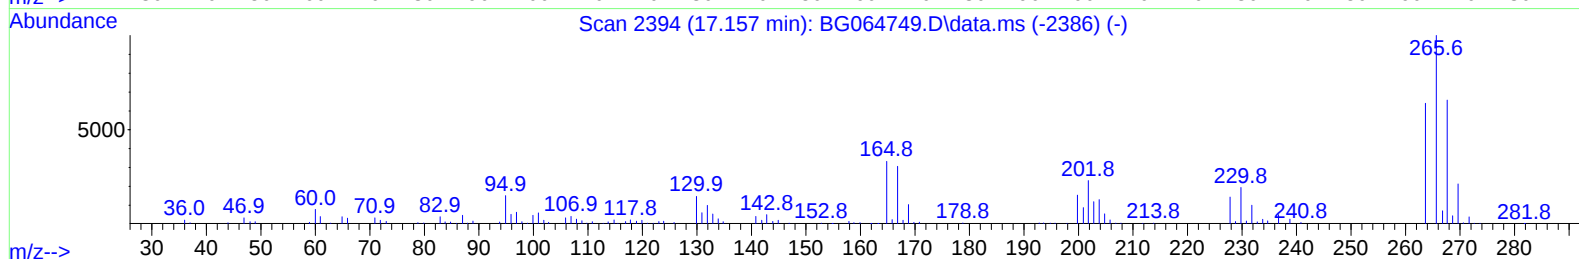
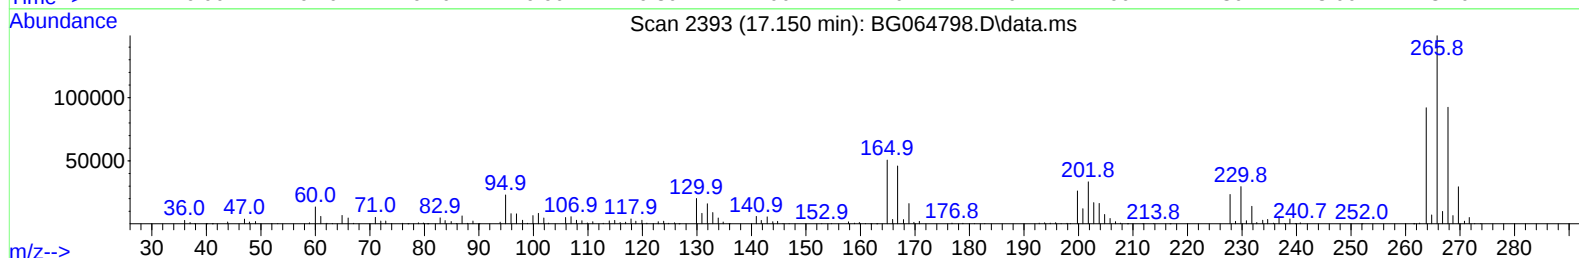


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064798.D
Acq On : 18 Nov 2025 11:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 12:05:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

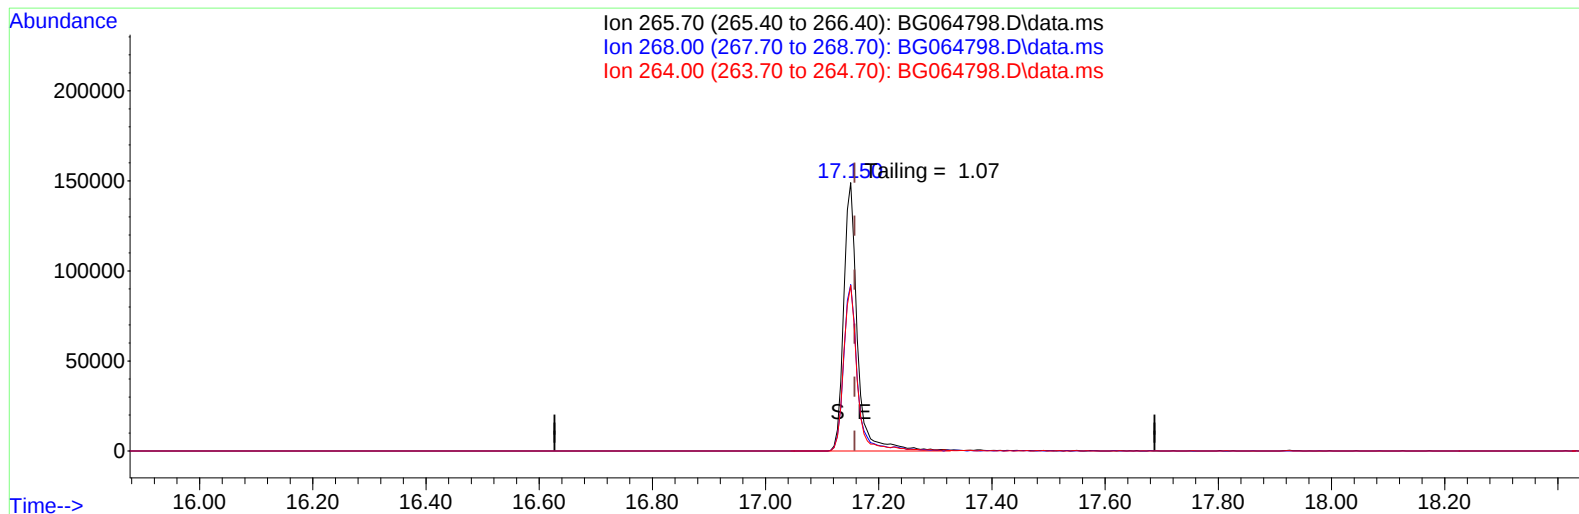

TIC: BG064798.D\data.ms

(70) Pentachlorophenol (C)




17.150min (-0.007) 33926.00 ng

response 250451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	66.50
264.00	64.00	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064798.D
Acq On : 18 Nov 2025 11:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 12:05:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

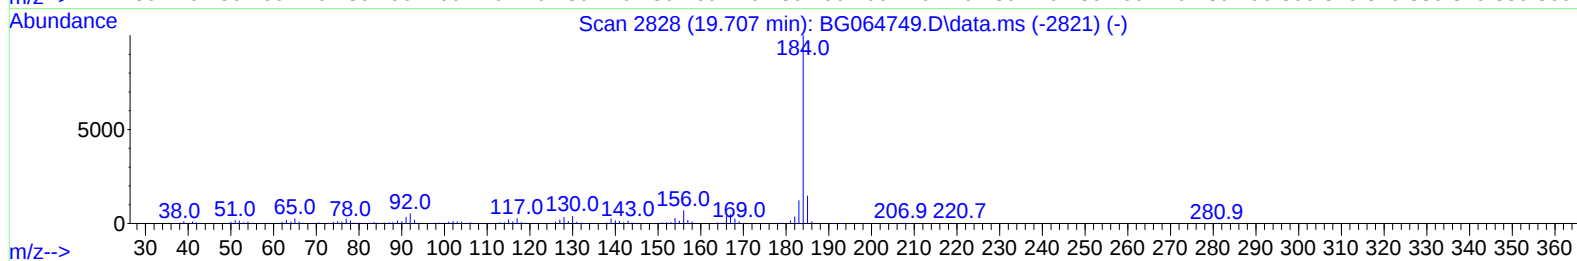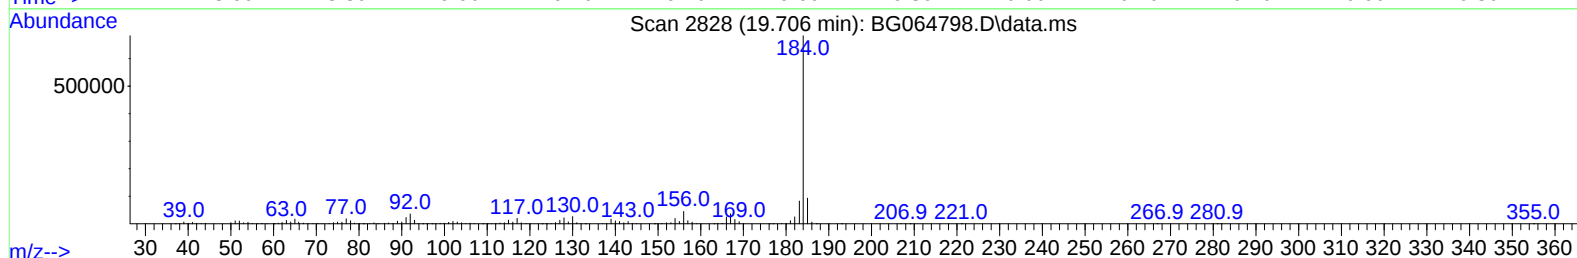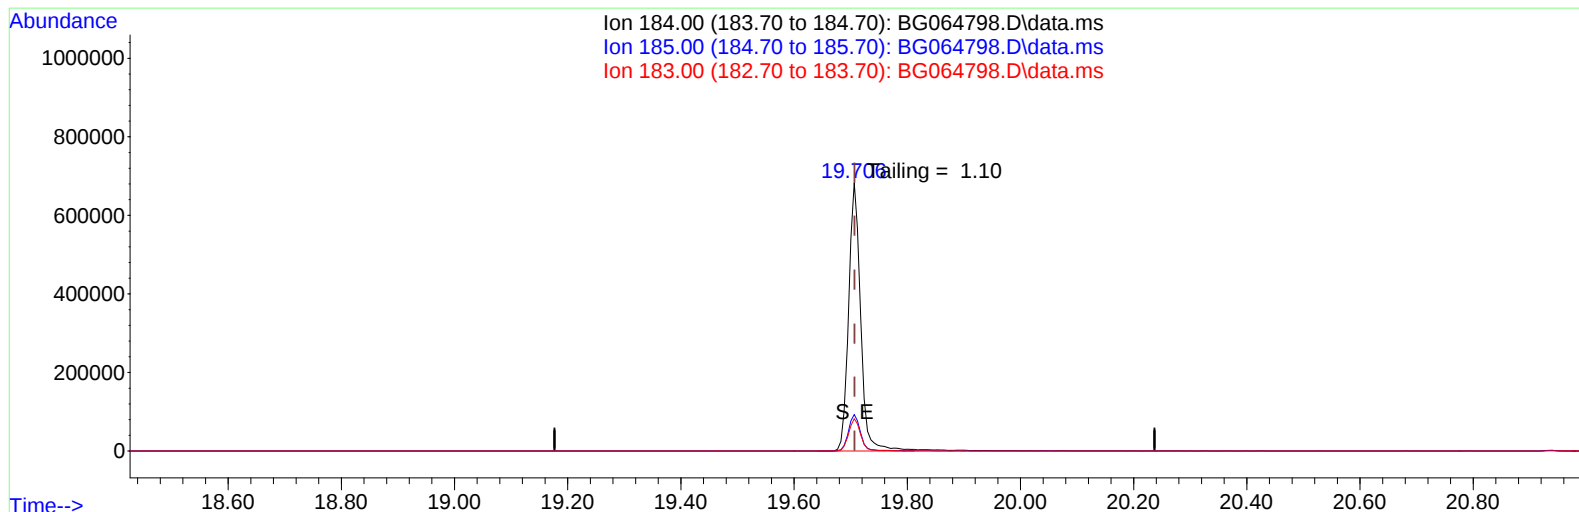

TIC: BG064798.D\data.ms

(77) Benzidine**19.706min (-0.000) 549166.45 ng****response 1019693**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.63
183.00	12.20	12.07
0.00	0.00	0.00