

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
 Data File : BG064803.D
 Acq On : 18 Nov 2025 14:59
 Operator : RC/JU
 Sample : Q3641-01RX
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-05-111325RX

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.135	3	8	18	rBV3	23739	48403	1.98%	0.491%
2	3.217	18	22	32	rVB	53575	85292	3.49%	0.866%
3	5.215	355	362	369	rBV	132952	211486	8.65%	2.147%
4	5.696	438	444	455	rBV	59513	98864	4.04%	1.004%
5	7.306	710	718	729	rBV	329138	607823	24.86%	6.172%
6	8.164	856	864	879	rVB	135049	244332	9.99%	2.481%
7	9.322	1053	1061	1072	rBV	223927	425762	17.42%	4.323%
8	10.978	1336	1343	1355	rBV	179200	349944	14.31%	3.553%
9	13.405	1748	1756	1771	rBV	700105	1191612	48.74%	12.100%
10	14.774	1981	1989	2003	rBV	354664	573842	23.47%	5.827%
11	16.108	2209	2216	2227	rBV	78574	137505	5.62%	1.396%
12	16.243	2231	2239	2250	rVV3	41756	76242	3.12%	0.774%
13	17.500	2446	2453	2459	rBV2	475147	778933	31.86%	7.909%
14	17.859	2508	2514	2523	rBV6	15457	32427	1.33%	0.329%
15	18.370	2595	2601	2608	rBV2	42500	80027	3.27%	0.813%
16	19.533	2793	2799	2807	rBV	85960	132673	5.43%	1.347%
17	19.891	2856	2860	2868	rVB	78431	130492	5.34%	1.325%
18	20.085	2887	2893	2902	rBV	1927210	2444772	100.00%	24.824%
19	20.385	2940	2944	2948	rVB4	18715	26327	1.08%	0.267%
20	21.378	3108	3113	3118	rBV2	81126	131623	5.38%	1.337%
21	21.748	3168	3176	3182	rBV	515828	964639	39.46%	9.795%
22	21.936	3206	3208	3215	rVB7	17105	24494	1.00%	0.249%
23	22.565	3311	3315	3320	rVB6	23422	49041	2.01%	0.498%
24	24.850	3697	3704	3710	rBV	22522	61062	2.50%	0.620%
25	25.003	3721	3730	3752	rVB	305197	940675	38.48%	9.552%




Sum of corrected areas: 9848292

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064803.D
Acq On : 18 Nov 2025 14:59
Operator : RC/JU
Sample : Q3641-01RX
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-05-111325RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

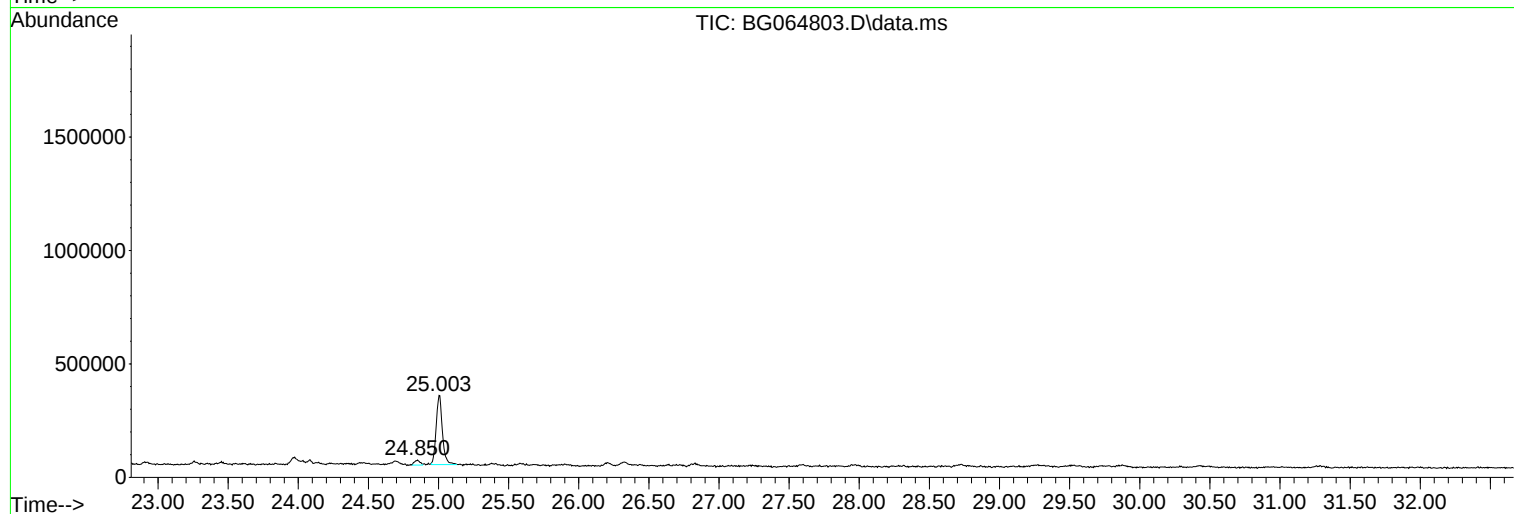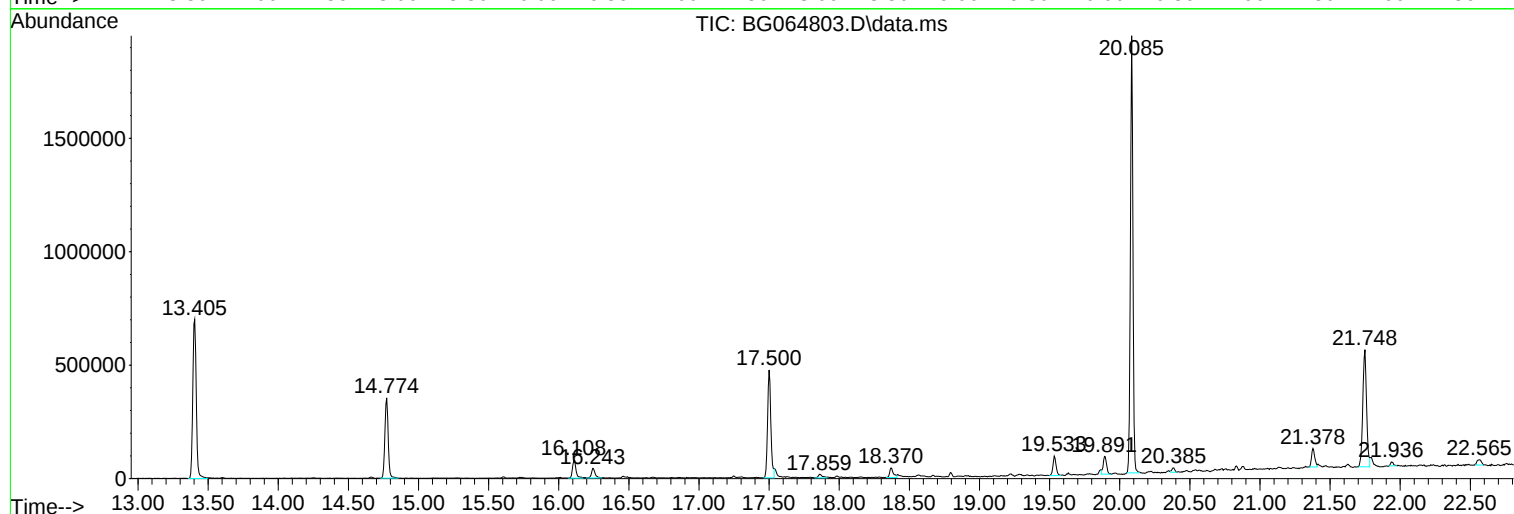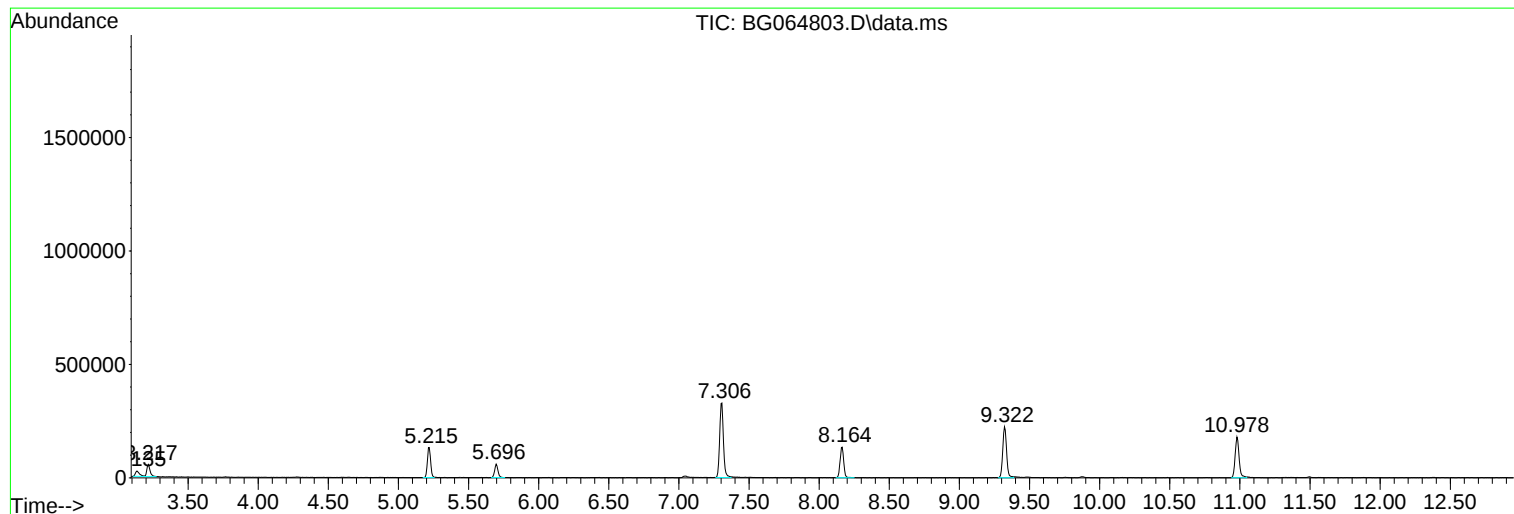

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064803.D
Acq On : 18 Nov 2025 14:59
Operator : RC/JU
Sample : Q3641-01RX
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-05-111325RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111825\
Data File : BG064803.D
Acq On : 18 Nov 2025 14:59
Operator : RC/JU
Sample : Q3641-01RX
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-05-111325RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------