
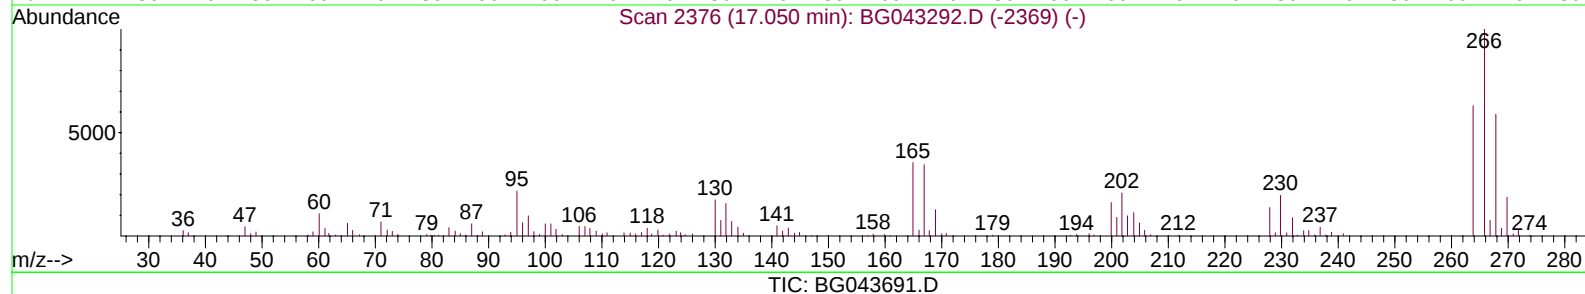
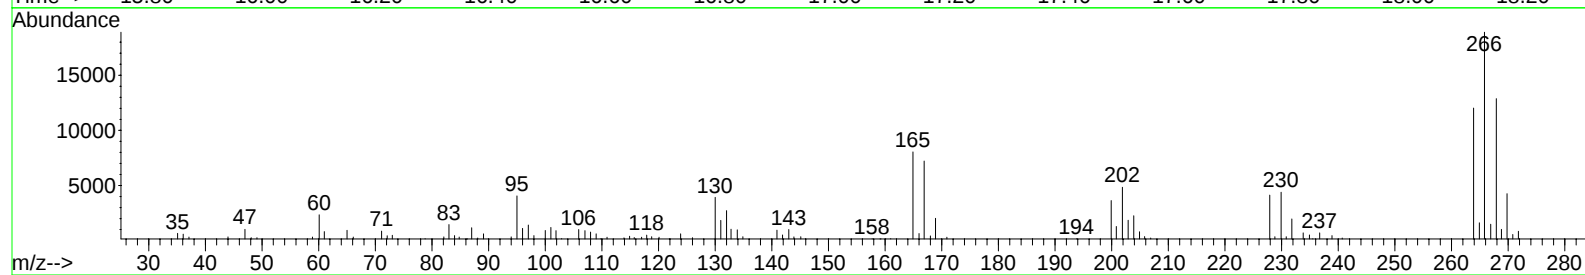


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111919\
Data File : BG043691.D
Acq On : 19 Nov 2019 10:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:45:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 15:23:15 2019
Response via : Initial Calibration

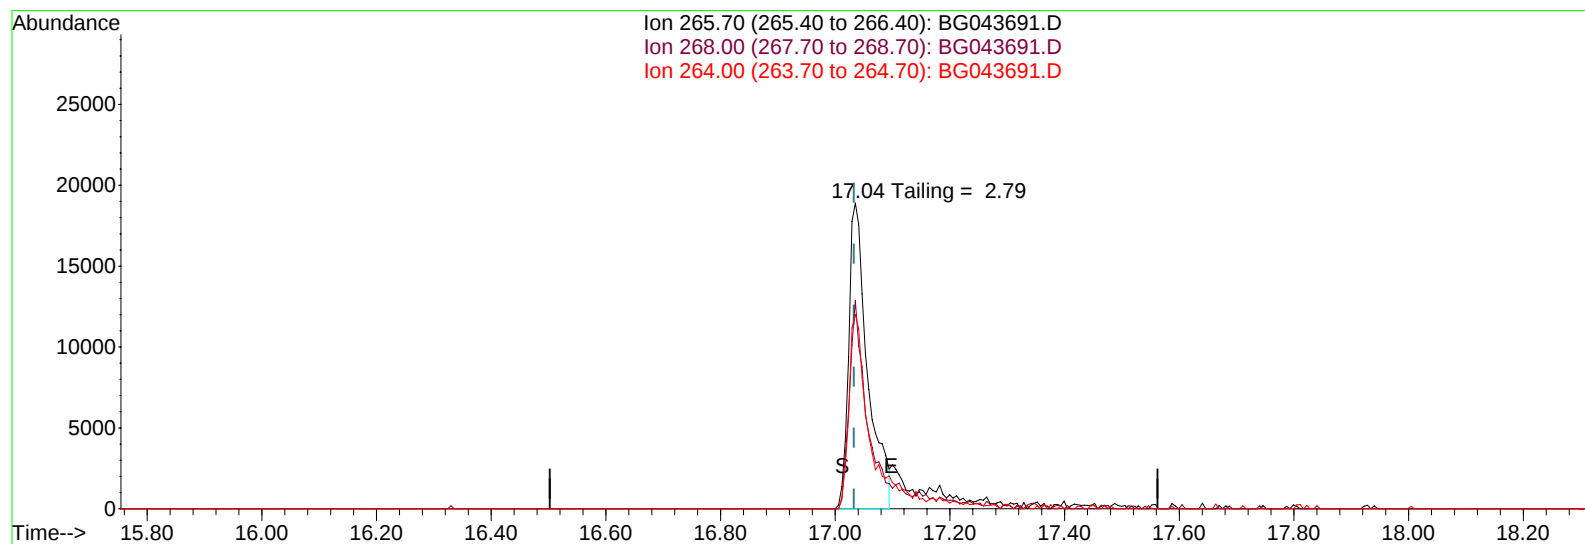

(70) Pentachlorophenol (C)




17.035min (+0.003) 34781.60ng

response 48231

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	68.10
264.00	61.10	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111919\
Data File : BG043691.D
Acq On : 19 Nov 2019 10:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:45:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 15:23:15 2019
Response via : Initial Calibration

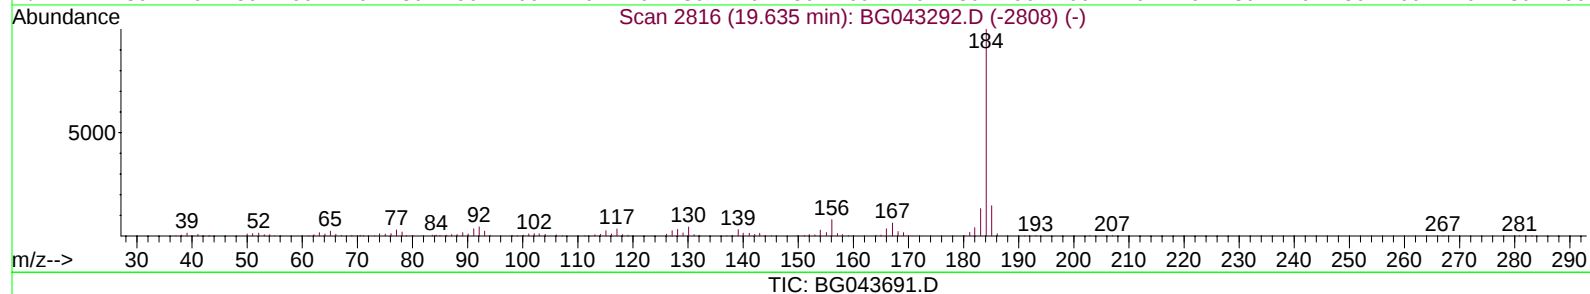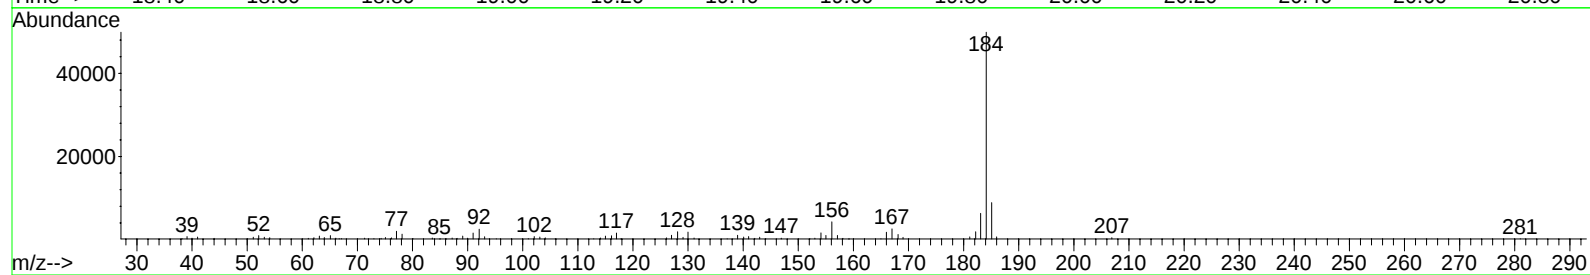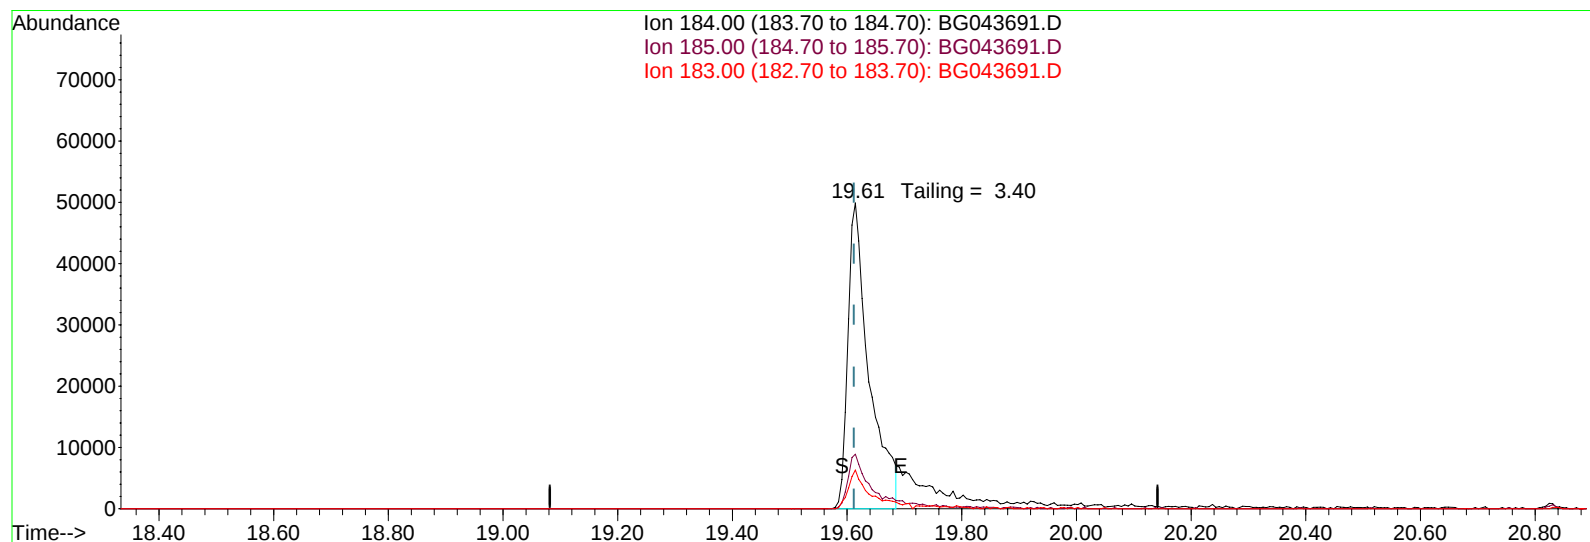

TIC: BG043691.D

(77) Benzidine

19.614min (+0.003) 0.00ng

response 151160

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	17.84
183.00	11.00	12.65
0.00	0.00	0.00