
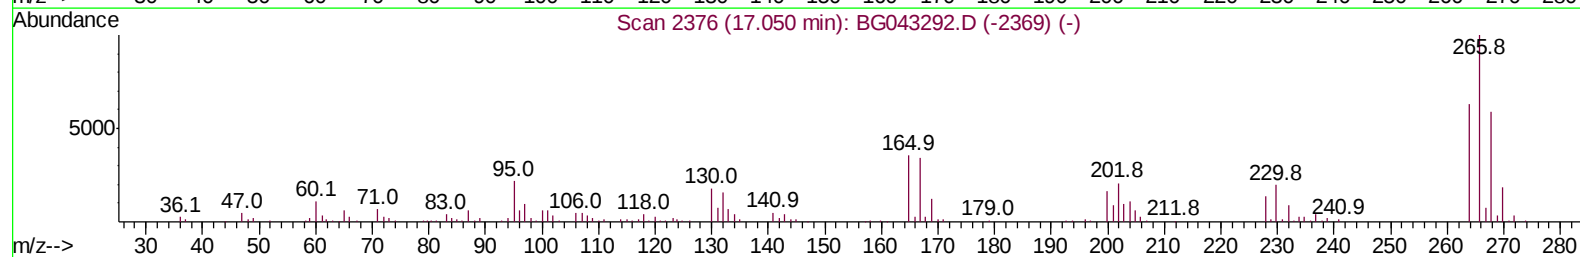
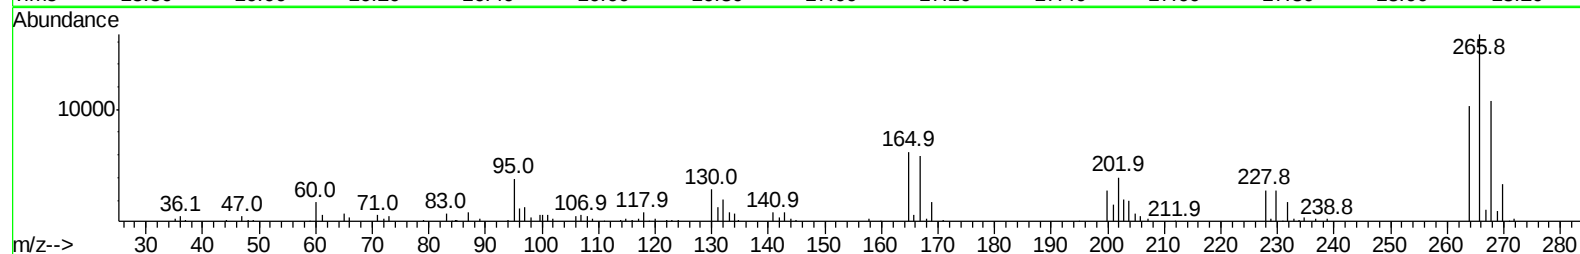


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111919\
Data File : BG043710.D
Acq On : 19 Nov 2019 23:28
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 03:26:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 15:23:15 2019
Response via : Initial Calibration

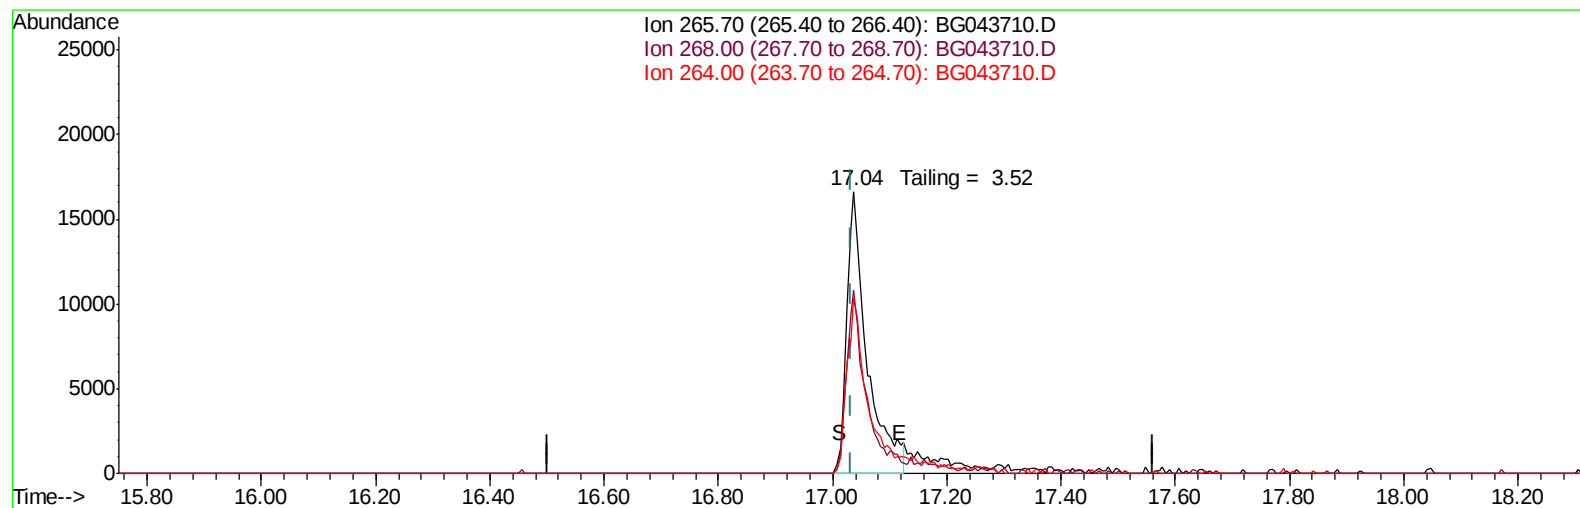

TIC: BG043710.D

(70) Pentachlorophenol (C)




17.037min (+0.005) 22584.86ng

response 43877

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.80
264.00	61.10	62.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111919\
Data File : BG043710.D
Acq On : 19 Nov 2019 23:28
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 03:26:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 15:23:15 2019
Response via : Initial Calibration

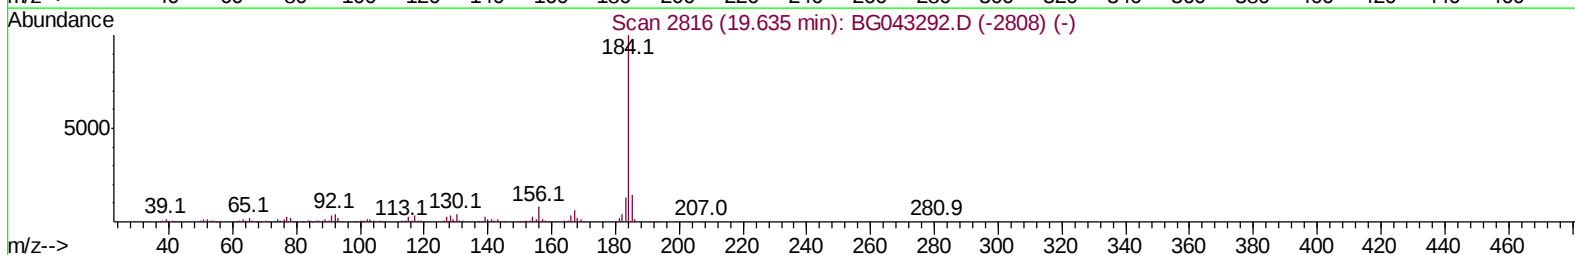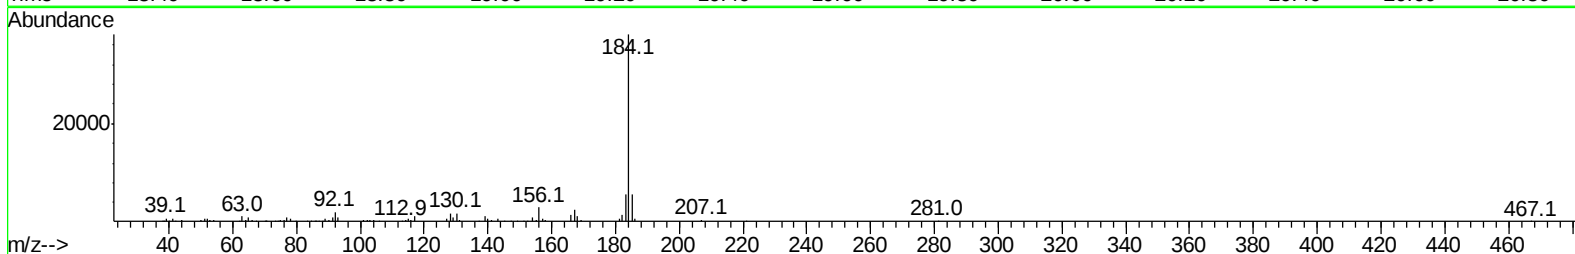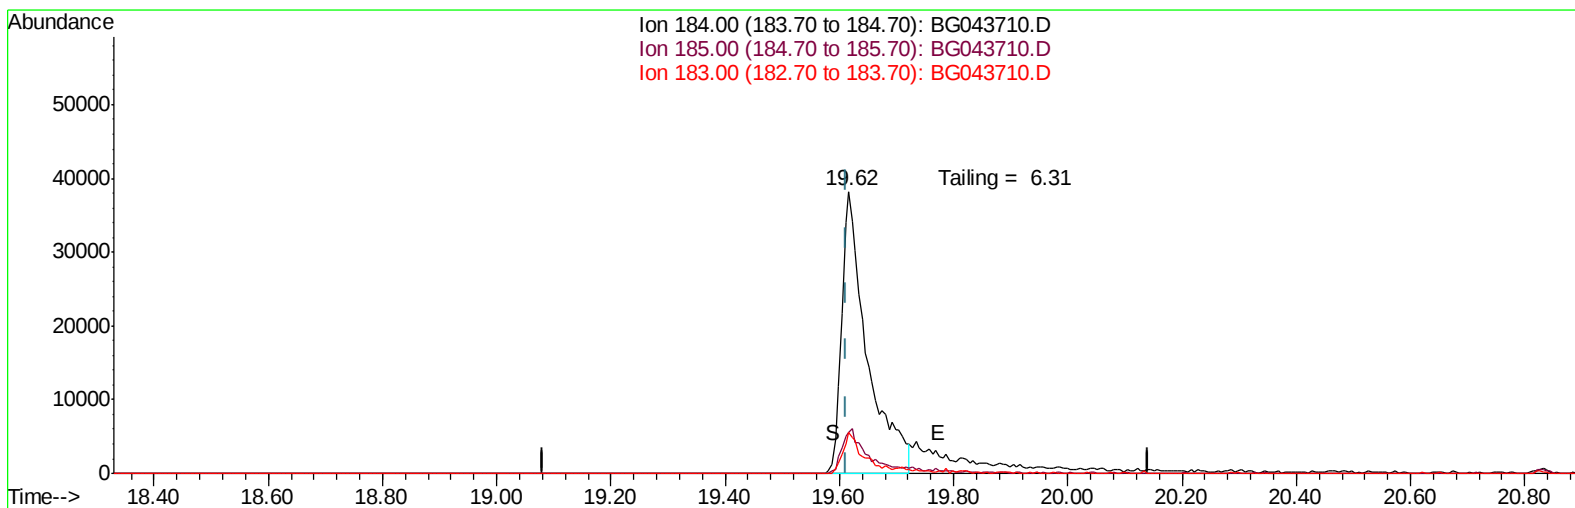

TIC: BG043710.D

(77) Benzidine

19.616min (+0.005) 0.00ng

response 119769

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.55
183.00	11.00	14.49#
0.00	0.00	0.00