


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111919\
 Data File : BG043710.D
 Acq On : 19 Nov 2019 23:28
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 19 15:23:15 2019

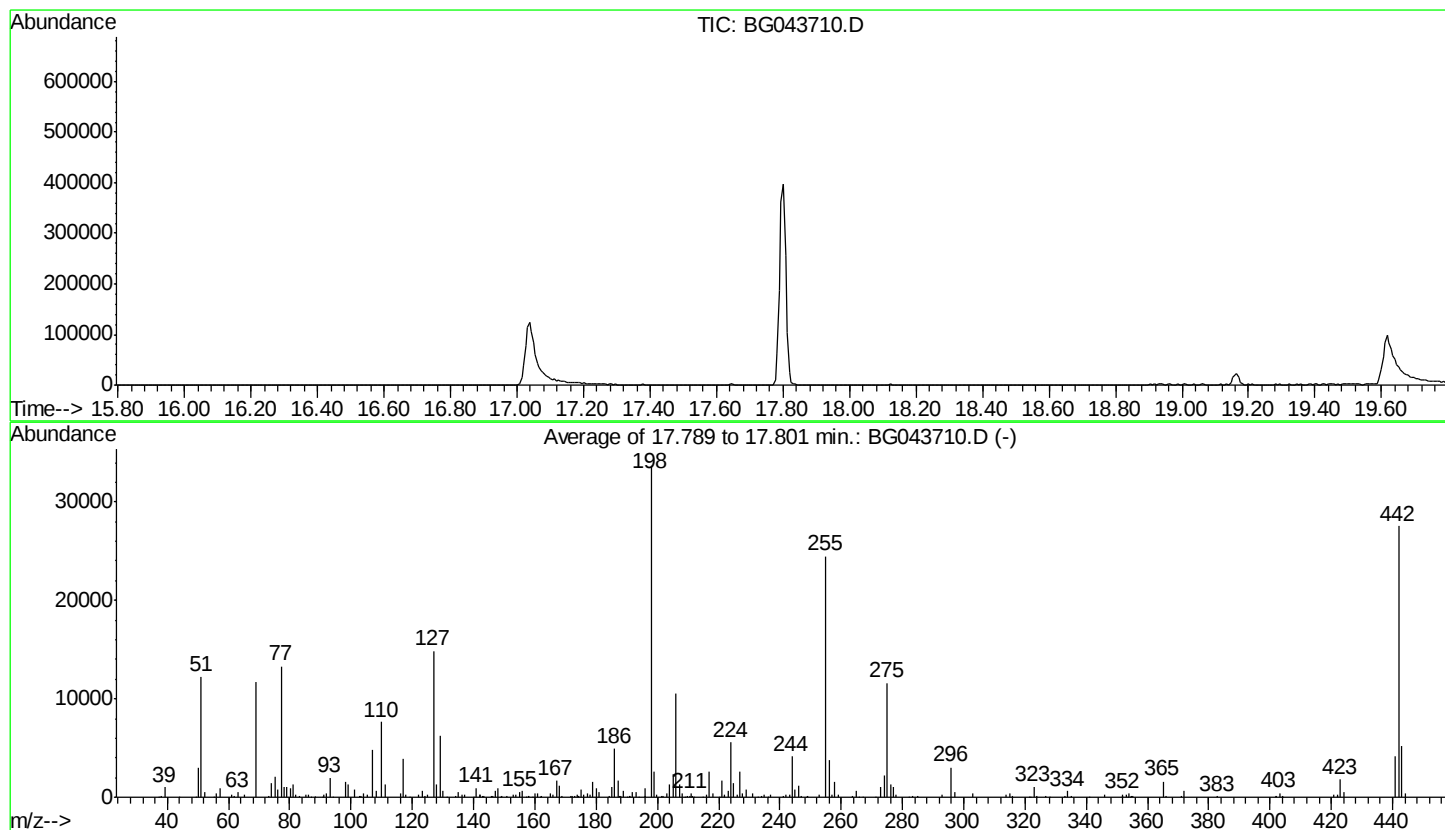

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	12227	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	11769	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	14875	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33685	PASS
199	198	5	9	7.7	2587	PASS
275	198	10	60	34.4	11603	PASS
365	198	1	100	4.7	1576	PASS
441	198	0.01	100	12.4	4191	PASS
442	198	50	100	81.7	27508	PASS
443	442	15	24	19.0	5229	PASS