

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
 Data File : BG047357.D
 Acq On : 19 Nov 2020 18:02
 Operator : CG/JU
 Sample : PB133052BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 20 04:02:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 19 14:25:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	37021	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	139766	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	119921	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	302209	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	329429	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	325980	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.61	96	5647	5.55	ng/uL	0.00
5) Phenol-d5	7.40	99	124711	33.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	75517	35.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	88864	35.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	95624	33.52	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	44861	38.86	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	50184	39.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	104217	36.13	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	131923	45.23	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	393019	38.18	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	442716	37.21	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	57413	36.55	ng/ul	0.00
58) Fluorene-d10	15.87	176	332960	35.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	59049	34.33	ng/ul	0.00
71) Anthracene-d10	17.72	188	579579	38.66	ng/ul	0.00
79) Pyrene-d10	19.98	212	702487	36.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	710674	37.88	ng/ul	0.00

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.96	70	3366	1.270	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
Data File : BG047357.D
Acq On : 19 Nov 2020 18:02
Operator : CG/JU
Sample : PB133052BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 20 04:02:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 19 14:25:26 2020
Response via : Initial Calibration

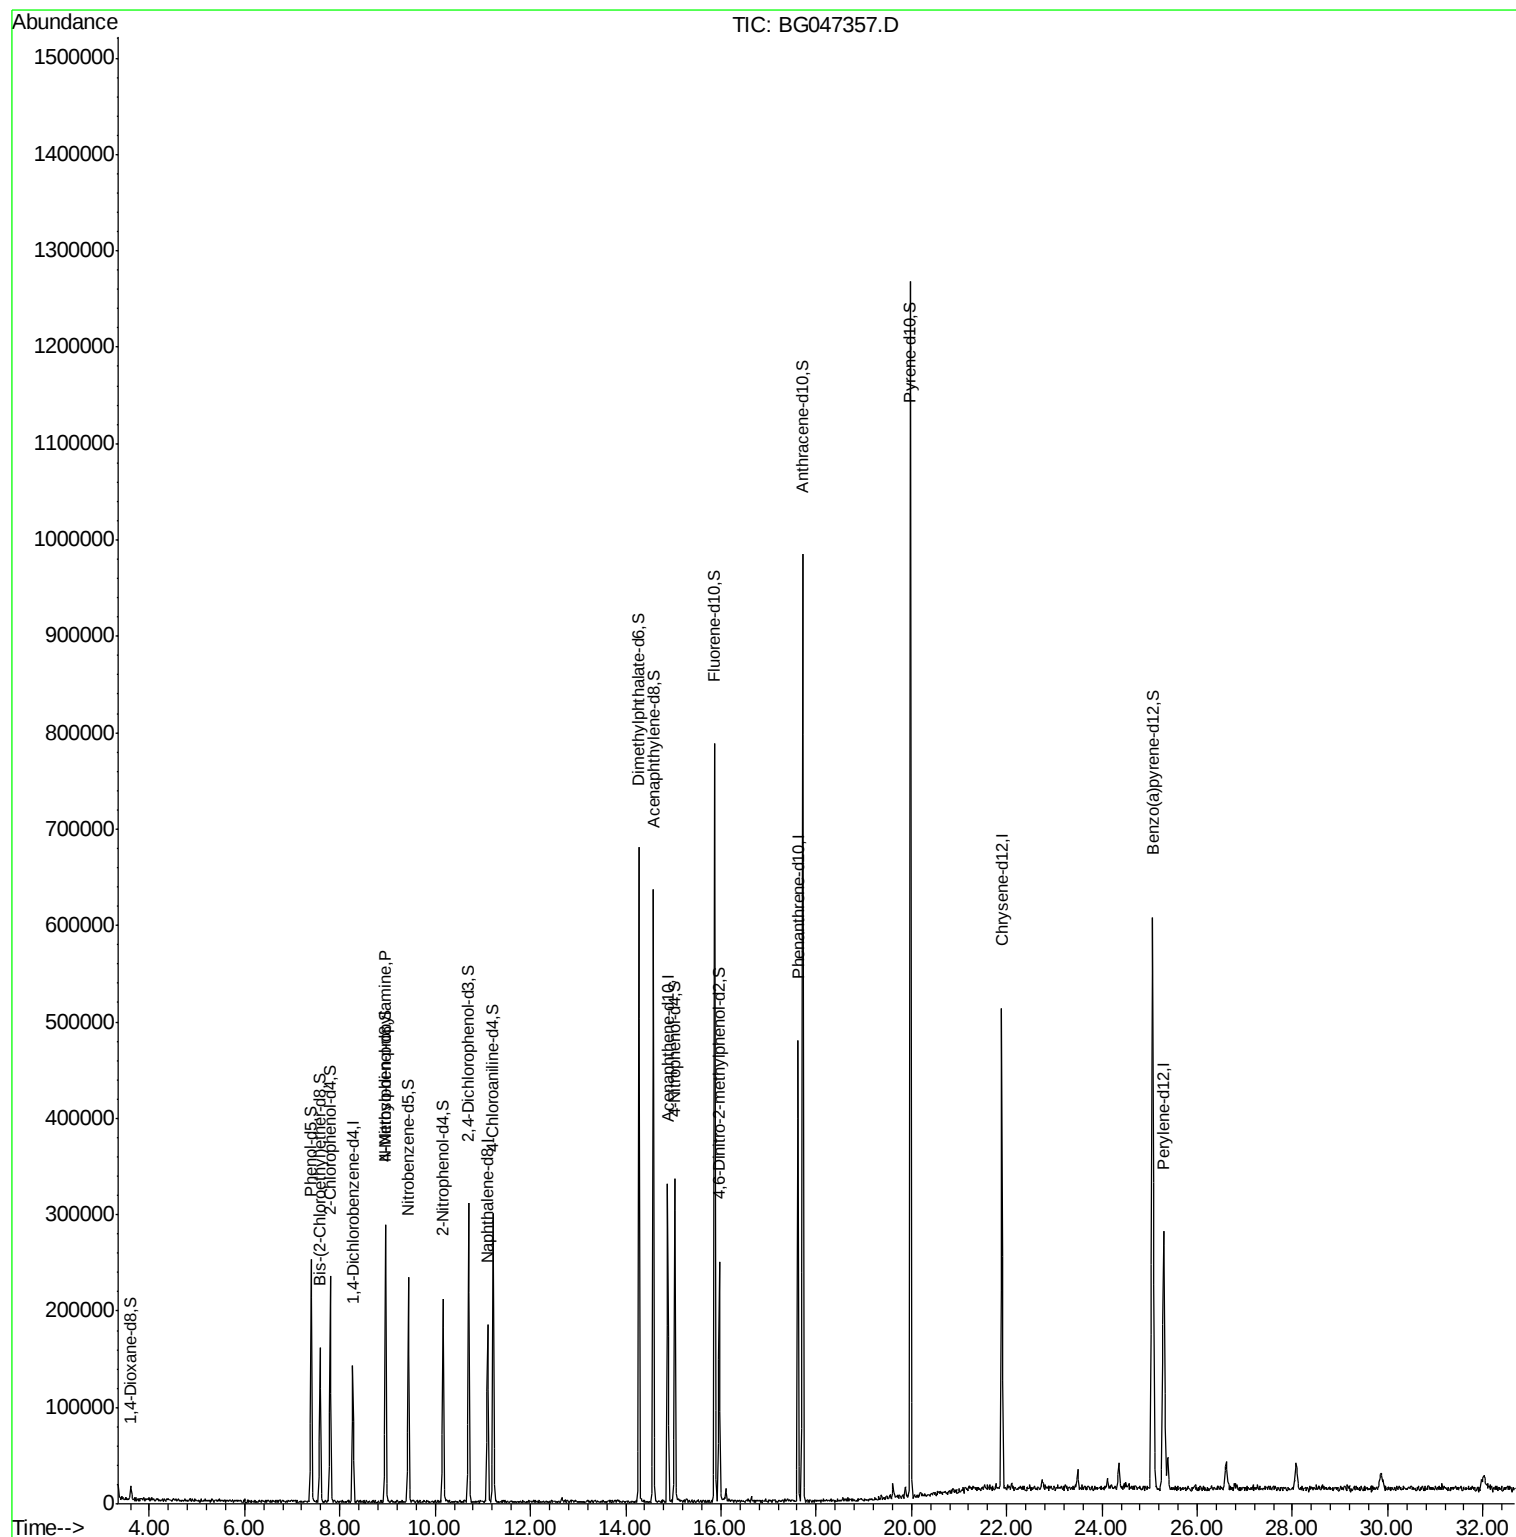

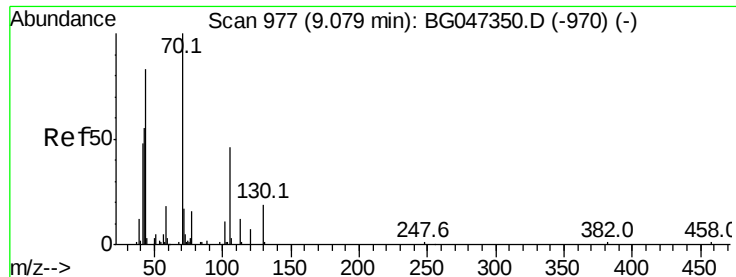

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.270 ng/ul
 RT: 8.96 min Scan# 956
 Delta R.T. -0.12 min
 Lab File: BG047357.D
 Acq: 19 Nov 2020 18:02

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	253.7	44.2	66.2#
101	0.0	9.0	13.6#
130	0.0	15.1	22.7#

