


#45
Dimethylphthalate
Concen: 6.460 ng/ul
RT: 14.32 min Scan# 1870
Delta R.T. -0.00 min
Lab File: BG047365.D
Acq: 19 Nov 2020 23:25

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.2
164	9.1	8.8	13.2



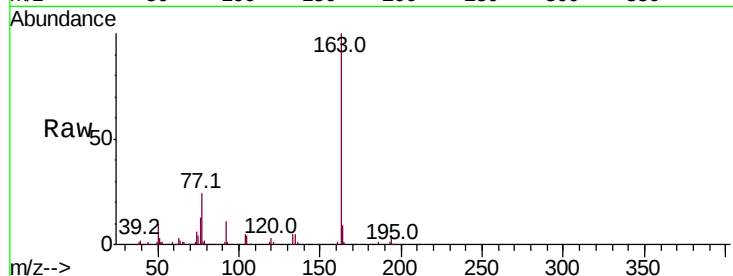


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

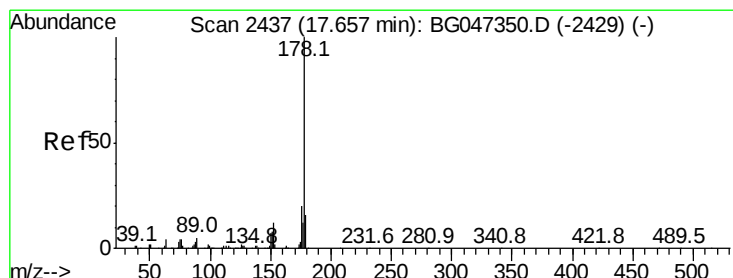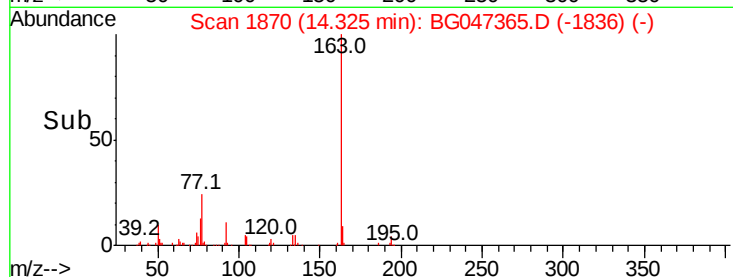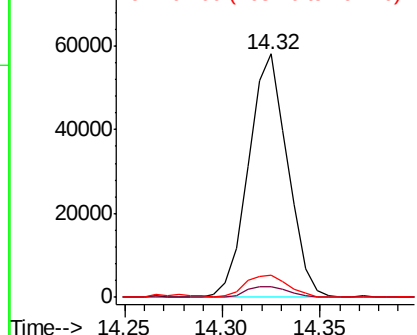

#70
Phenanthrene
Concen: 1.666 ng/ul
RT: 17.66 min Scan# 2438
Delta R.T. 0.01 min
Lab File: BG047365.D
Acq: 19 Nov 2020 23:25

Tgt Ion	Ratio	Lower	Upper
178	100		
179	12.5	12.8	19.2#
176	20.6	15.7	23.5

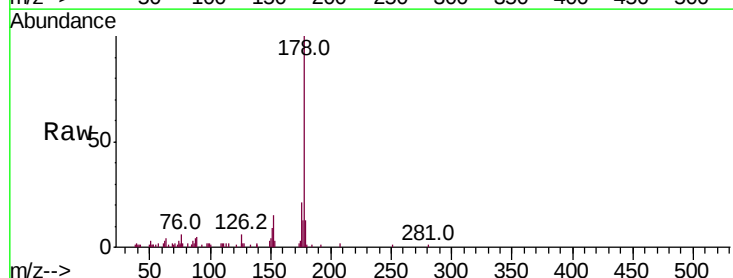

Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

