

#45

Dimethylphthalate

Concen: 7.550 ng/ul

RT: 14.32 min Scan# 1870

Delta R.T. -0.00 min

Lab File: BG047367.D

Acq: 20 Nov 2020 00:46

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 97573

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2




164 10.7 8.8 13.2

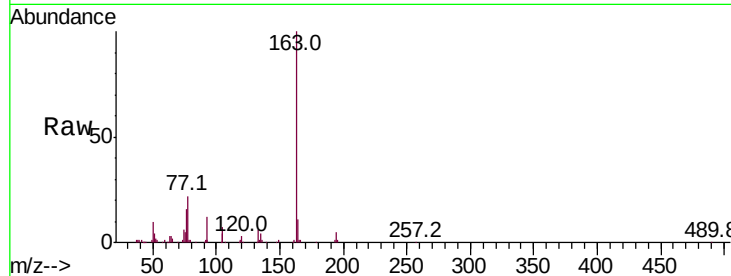

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

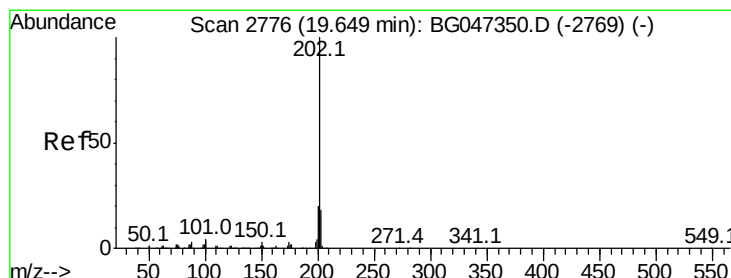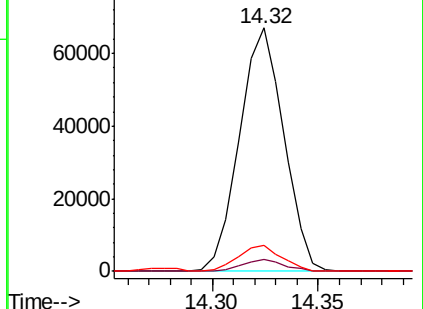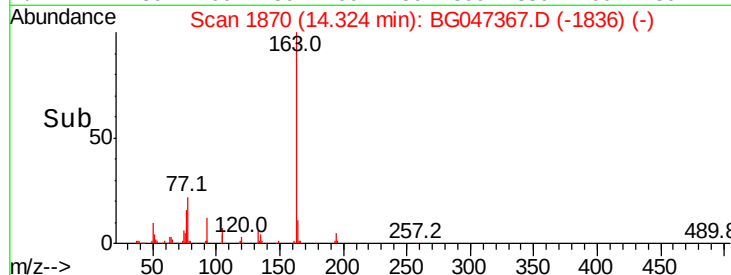

#77

Fluoranthene

Concen: 1.299 ng/ul

RT: 19.65 min Scan# 2776

Delta R.T. -0.00 min

Lab File: BG047367.D

Acq: 20 Nov 2020 00:46


Tgt Ion:202 Resp: 30877

Ion Ratio Lower Upper

202 100

101 4.4 3.3 4.9

100 3.1 3.4 5.0#

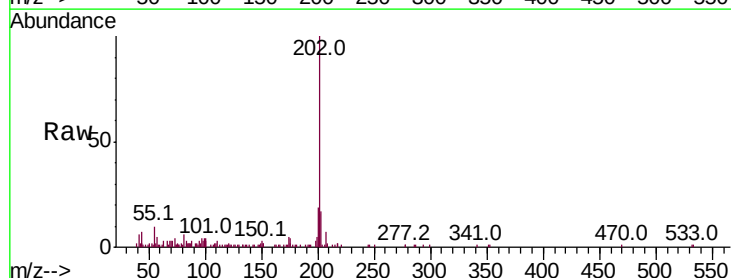

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

