

#45

Dimethylphthalate

Concen: 7.104 ng/ul

RT: 14.32 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG047368.D

Acq: 20 Nov 2020 1:26

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 89890

Ion Ratio Lower Upper

163 100

194 3.4 3.4 5.2#




164 9.4 8.8 13.2

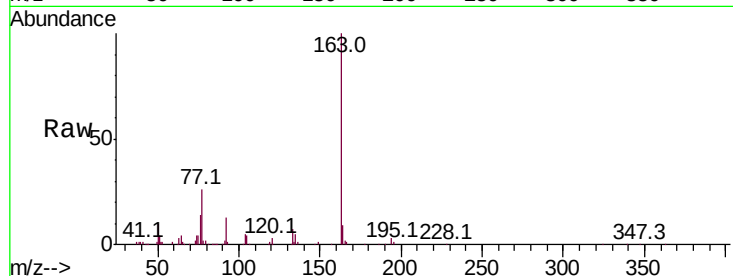

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

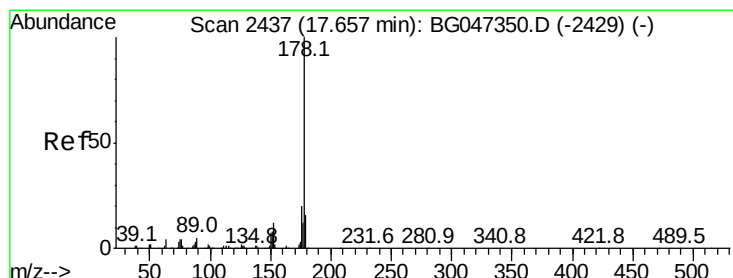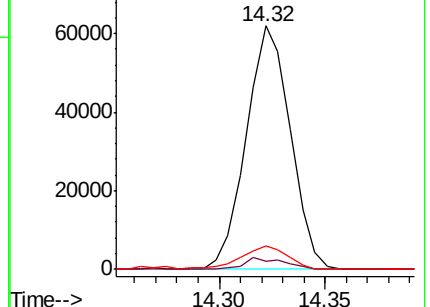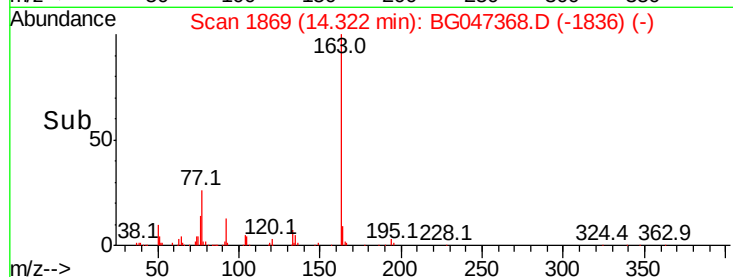

#70

Phenanthrene

Concen: 2.491 ng/ul

RT: 17.66 min Scan# 2437

Delta R.T. 0.00 min

Lab File: BG047368.D

Acq: 20 Nov 2020 1:26


Tgt Ion:178 Resp: 45443

Ion Ratio Lower Upper

178 100

179 16.1 12.8 19.2

176 19.8 15.7 23.5

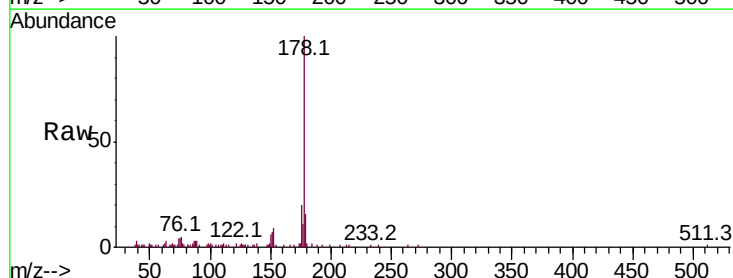

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

