

#72

Anthracene

Concen: 2.474 ng/ul

RT: 17.66 min Scan# 2437

Delta R.T. -0.09 min

Lab File: BG047368.D

Acq: 20 Nov 2020 1:26

Instrument :

BNA_G

ClientSampleId :


Tot Ion:178 Resp: 45443

Ion Ratio Lower Upper




178 100

179 16.1 12.2 18.2

176 19.8 16.2 24.4

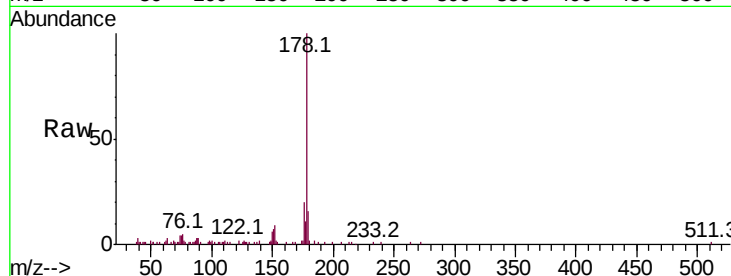

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

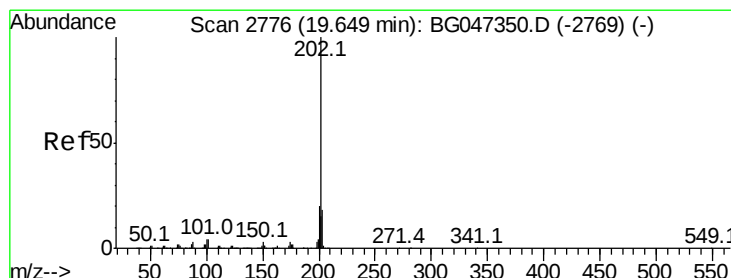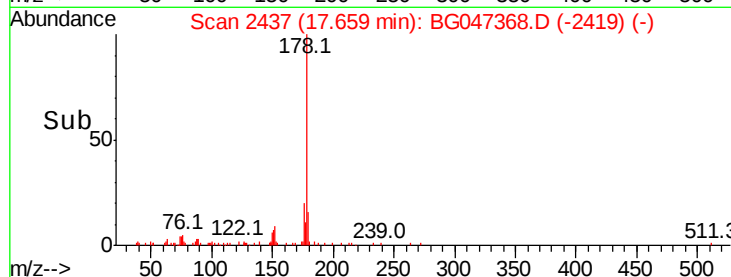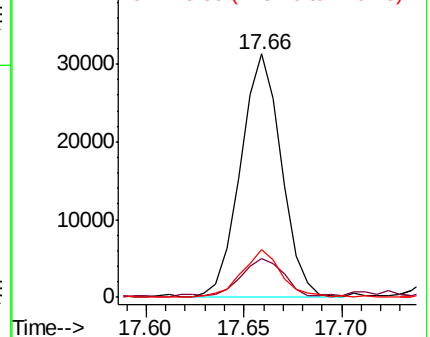

#77

Fluoranthene

Concen: 4.807 ng/ul

RT: 19.65 min Scan# 2776

Delta R.T. 0.00 min

Lab File: BG047368.D

Acq: 20 Nov 2020 1:26


Tgt Ion:202 Resp: 110738

Ion Ratio Lower Upper

202 100

101 3.8 3.3 4.9

100 3.0 3.4 5.0#

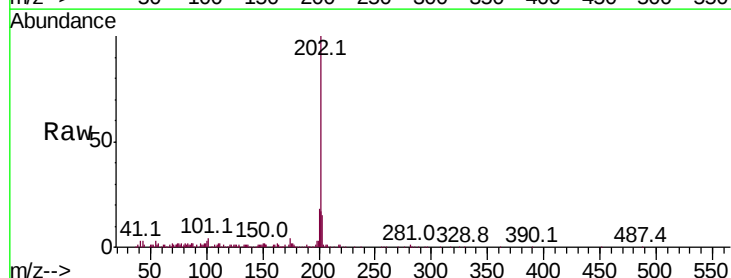

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

