

#17

Hexachloroethane

Concen: 18.703 ng/ul

RT: 9.37 min Scan# 1027

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08

Instrument :

BNA_G

ClientSampleId :


Tot Ion:117 Resp: 27314

Ion Ratio Lower Upper

117 100

201 127.6 96.2 144.4




199 80.3 63.0 94.4

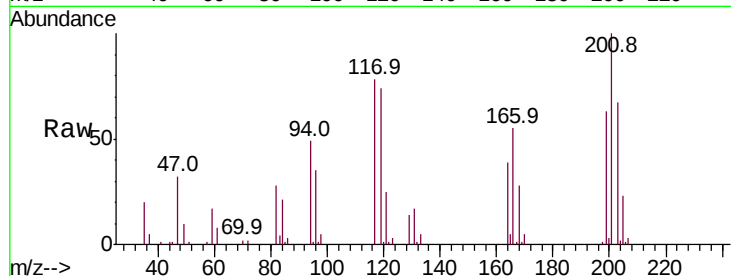

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

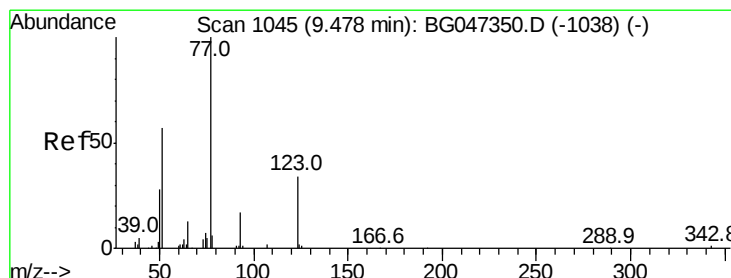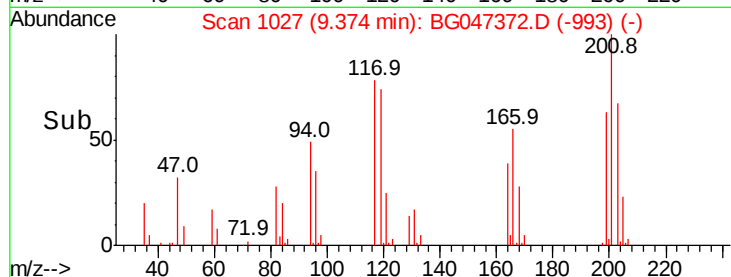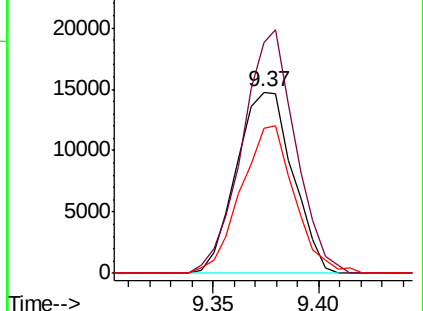

#20

Nitrobenzene

Concen: 19.239 ng/ul

RT: 9.49 min Scan# 1046

Delta R.T. 0.01 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08


Tgt Ion: 77 Resp: 91097

Ion Ratio Lower Upper

77 100

123 38.7 27.3 40.9

65 14.5 10.4 15.6

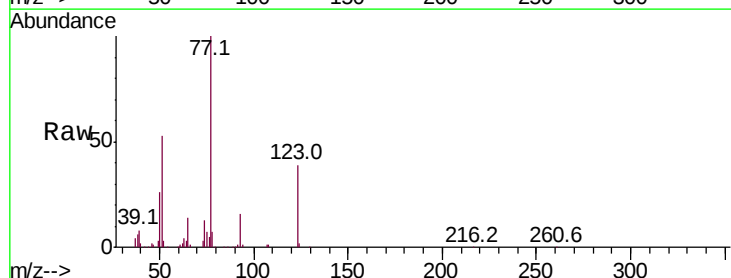

Abundance Ion 77.00 (76.70 to 77.70): BGC

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BGC

