
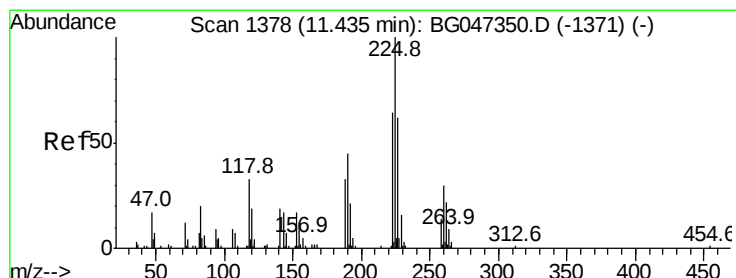
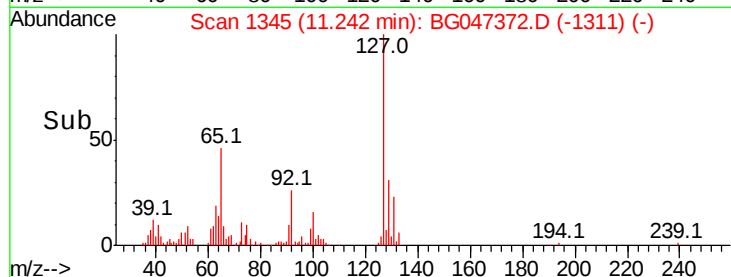
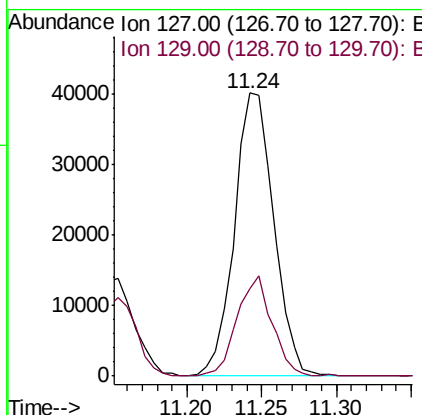


#30
4-Chloroaniline
Concen: 20.969 ng/ul
RT: 11.24 min Scan# 1345
Delta R.T. 0.00 min
Lab File: BG047372.D
Acq: 20 Nov 2020 4:08

Instrument :
BNA_G
ClientSampleId :

Tot Ion:127 Resp: 73917
Ion Ratio Lower Upper
127 100
129 30.8 20.1 30.1#

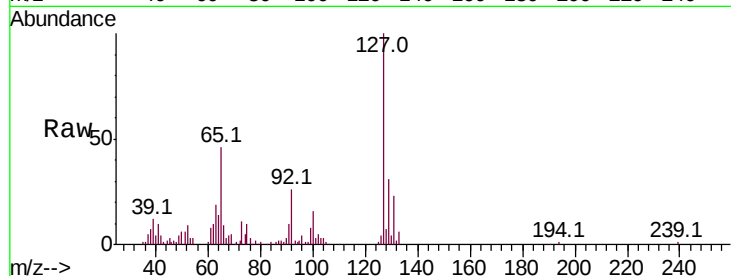

#31
Hexachlorobutadiene
Concen: 20.442 ng/ul
RT: 11.44 min Scan# 1378
Delta R.T. 0.00 min
Lab File: BG047372.D
Acq: 20 Nov 2020 4:08

Tgt Ion:225 Resp: 62449
Ion Ratio Lower Upper
225 100
223 58.7 51.0 76.6
227 58.9 47.0 70.6

