

#59

Fluorene

Concen: 19.158 ng/ul

RT: 15.93 min Scan# 2142

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08

Instrument :

BNA_G

ClientSampleId :


Tot Ion:166 Resp: 219134

Ion Ratio Lower Upper




166 100

165 94.5 79.0 118.4

167 14.0 10.4 15.6

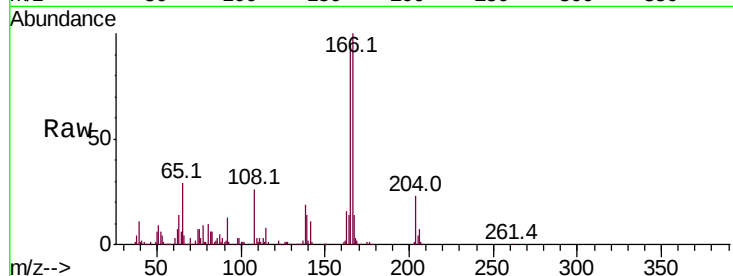

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

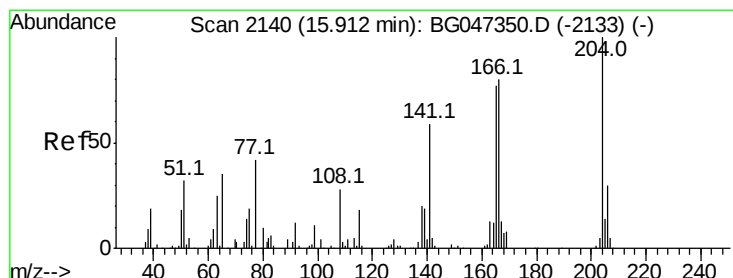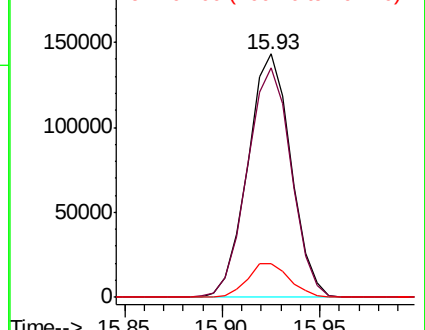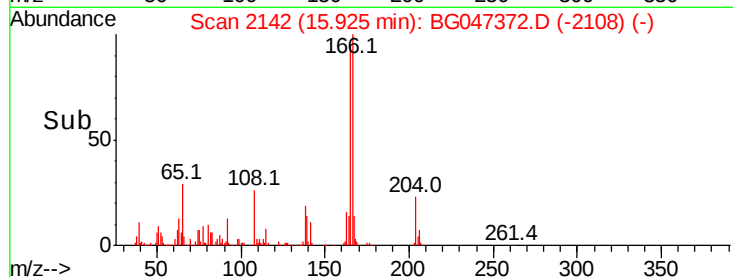

#60

4-Chlorophenyl-phenylether

Concen: 19.070 ng/ul

RT: 15.91 min Scan# 2140

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08


Tgt Ion:204 Resp: 131023

Ion Ratio Lower Upper

204 100

206 33.6 24.1 36.1

141 55.1 47.0 70.4

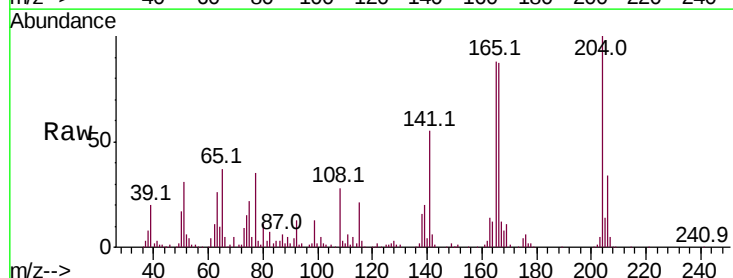

Abundance Ion 204.00 (203.70 to 204.70): E
Ion 206.00 (205.70 to 206.70): E
Ion 141.00 (140.70 to 141.70): E

