

#61

4-Nitroaniline

Concen: 18.895 ng/ul

RT: 15.93 min Scan# 2142

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08

Instrument :

BNA_G

ClientSampled :


Tot Ion:138 Resp: 41402

Ion Ratio Lower Upper

138 100

92 66.0 50.8 76.2




108 135.7 102.6 154.0

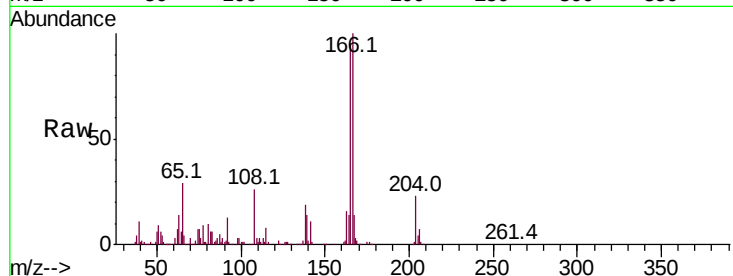

Abundance Ion 138.00 (137.70 to 138.70): E

Ion 92.00 (91.70 to 92.70): BG

Ion 108.00 (107.70 to 108.70): E

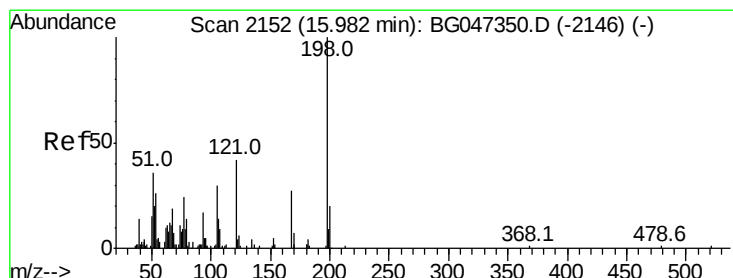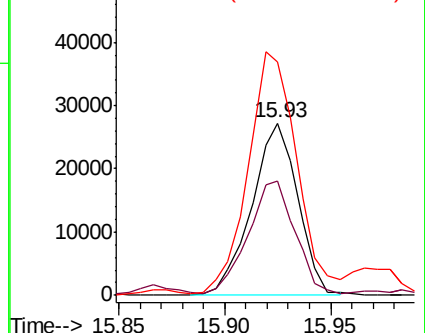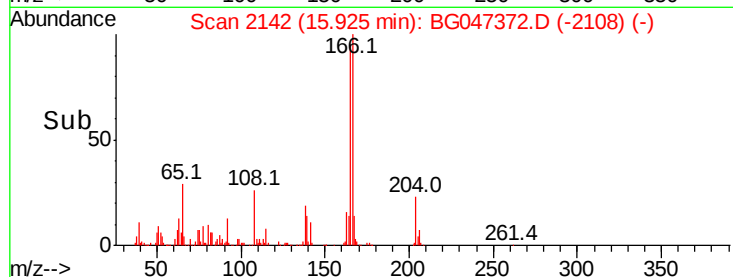

#64

4,6-Dinitro-2-methylphenol

Concen: 18.273 ng/ul

RT: 15.98 min Scan# 2152

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08


Tgt Ion:198 Resp: 39061

Ion Ratio Lower Upper

198 100

182 4.2 3.0 4.6

77 32.3 20.8 31.2#

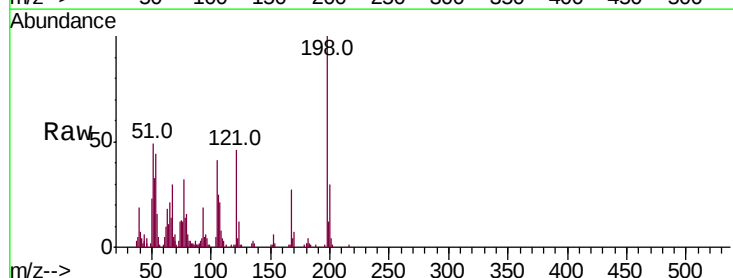

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): BG

