

#67

Hexachlorobenzene

Concen: 20.781 ng/ul

RT: 16.92 min Scan# 2312

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08

Instrument :

BNA_G

ClientSampleId :


Tot Ion:284 Resp: 99108

Ion Ratio Lower Upper

284 100

142 26.1 23.8 35.6




249 29.5 24.2 36.4

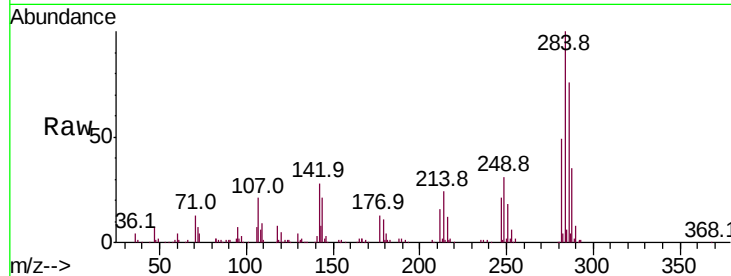

Abundance Ion 284.00 (283.70 to 284.70): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

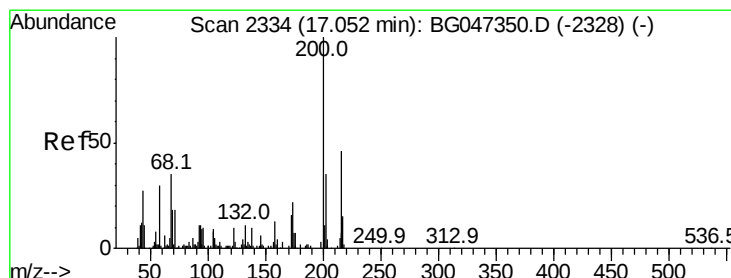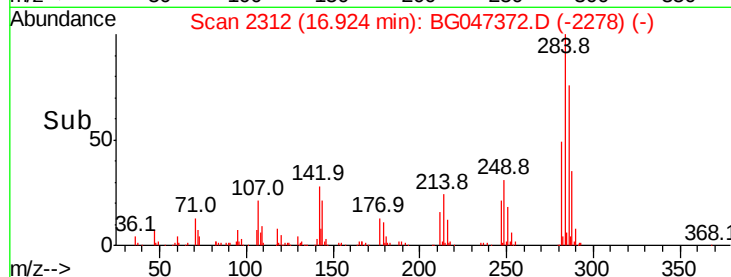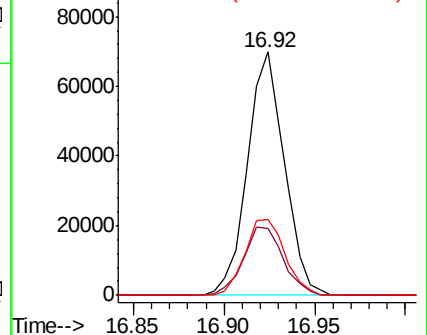

#68

Atrazine

Concen: 19.087 ng/ul

RT: 17.05 min Scan# 2334

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08


Tgt Ion:200 Resp: 86059

Ion Ratio Lower Upper

200 100

173 20.6 17.5 26.3

215 51.0 36.5 54.7

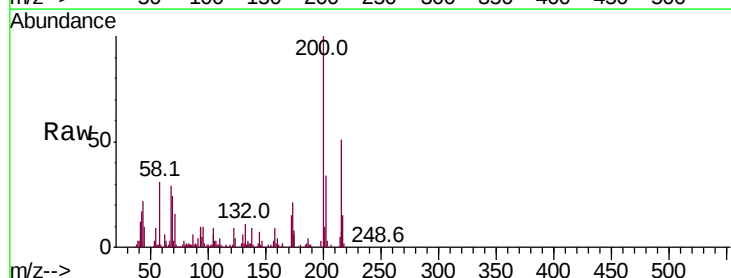

Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

