

#82

3,3'-Dichlorobenzidine

Concen: 19.272 ng/ul

RT: 21.78 min Scan# 3139

Delta R.T. 0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08

Instrument :

BNA_G

ClientSampleId :


Tot Ion:252 Resp: 148725

Ion Ratio Lower Upper

252 100

254 63.6 54.0 81.0




126 4.9 5.2 7.8#

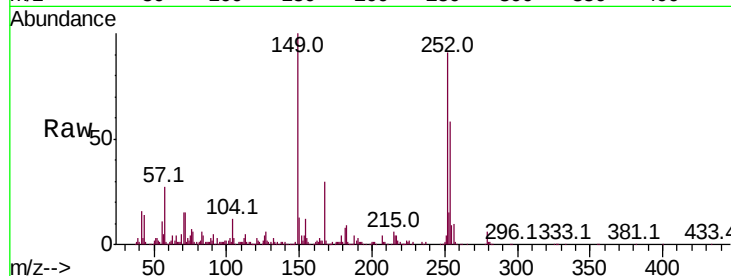

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

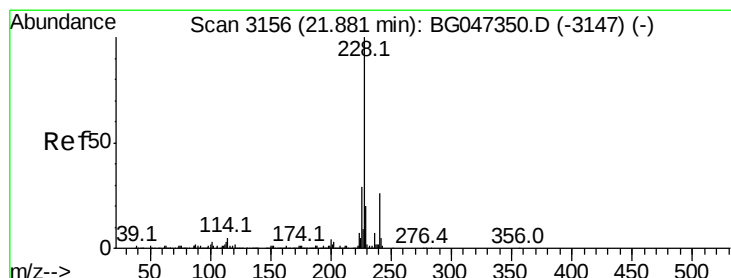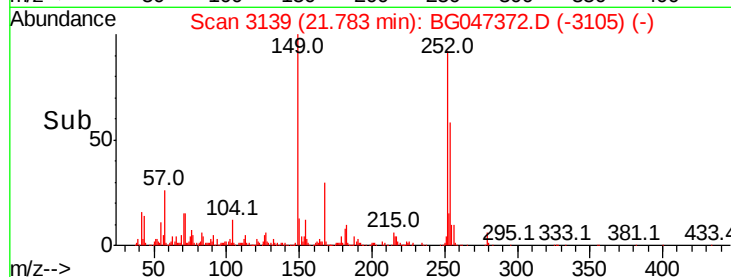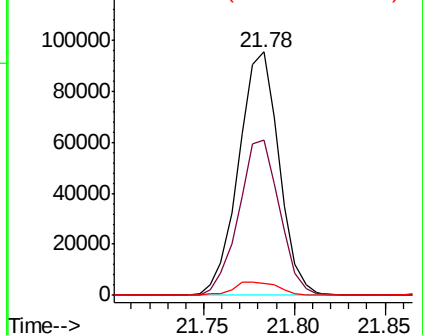

#83

Benzo(a)anthracene

Concen: 19.158 ng/ul

RT: 21.88 min Scan# 3155

Delta R.T. -0.00 min

Lab File: BG047372.D

Acq: 20 Nov 2020 4:08


Tgt Ion:228 Resp: 450593

Ion Ratio Lower Upper

228 100

229 19.7 16.2 24.2

226 27.2 23.3 34.9

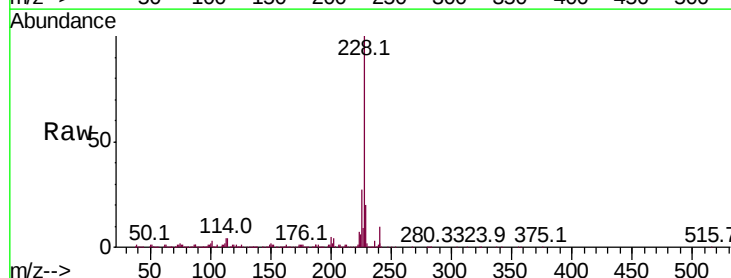

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

