
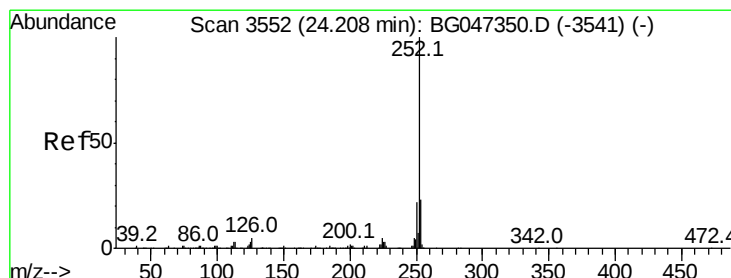
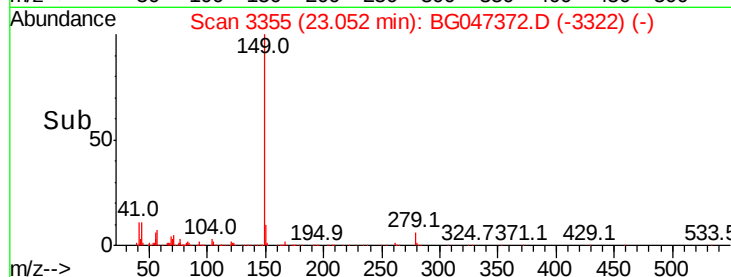
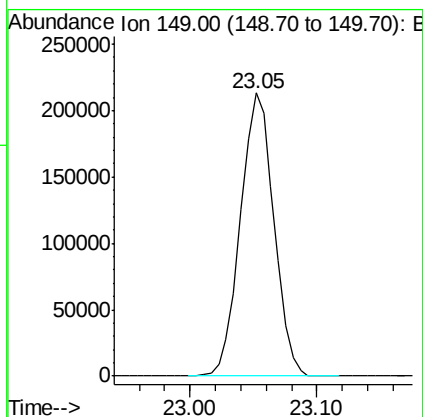


#87
 Di-n-octyl phthalate
 Concen: 19.541 ng/ul
 RT: 23.05 min Scan# 3355
 Delta R.T. -0.00 min
 Lab File: BG047372.D
 Acq: 20 Nov 2020 4:08

Instrument :
 BNA_G
 ClientSampleId :

Tgt Ion:149 Resp: 389671

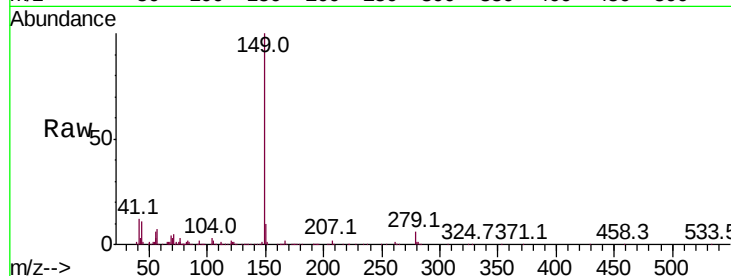

#88
 Benzo(b)fluoranthene
 Concen: 18.598 ng/ul
 RT: 24.22 min Scan# 3553
 Delta R.T. 0.01 min
 Lab File: BG047372.D
 Acq: 20 Nov 2020 4:08

Tgt Ion:252 Resp: 472776

Ion	Ratio	Lower	Upper
252	100		
253	22.0	18.4	27.6
125	3.0	2.5	3.7

