

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
 Data File : BG047368.D
 Acq On : 20 Nov 2020 1:26
 Operator : CG/JU
 Sample : L4710-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AW5

Manual Integrations
 APPROVED

mohammad
 11/23/2020 1:29:01 PM

Quant Time: Nov 20 07:38:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 19 14:25:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	48454	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	192996	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	144501	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	337763	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	291963	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	317570	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.61	96	2521	1.89	ng/uL	0.00
5) Phenol-d5	7.40	99	65655	13.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	38155	13.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	46396	14.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	38971	10.44	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	24433	15.33	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	27775	15.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	56831	14.27	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	54414	13.51	ng/ul	0.00
44) Dimethylphthalate-d6	14.27	166	196277	15.82	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	230898	16.11	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	30674	16.21	ng/ul	0.00
58) Fluorene-d10	15.87	176	174367	15.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	28636	14.89	ng/ul	0.00
71) Anthracene-d10	17.72	188	297071	17.73	ng/ul	0.00
79) Pyrene-d10	19.98	212	342588	20.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.07	264	359948	19.69	ng/ul	0.00

Target Compounds

					Ovalue	
45) Dimethylphthalate	14.32	163	89890	7.104	ng/ul#	96
70) Phenanthrene	17.66	178	45443	2.491	ng/ul	100
77) Fluoranthene	19.65	202	110738	4.807	ng/ul#	98
80) Pyrene	20.01	202	90266	4.365	ng/ul	98
83) Benzo(a)anthracene	21.88	228	47513	2.287	ng/ul	93
84) Bis(2-ethylhexyl)phthalate	21.78	149	327111	32.308	ng/ul	98
85) Chrysene	21.94	228	55910	2.828	ng/ul	98
88) Benzo(b)fluoranthene	24.21	252	83293m	3.715	ng/ul	
89) Benzo(k)fluoranthene	24.27	252	29325m	1.327	ng/ul	
91) Benzo(a)pyrene	25.14	252	55061	2.755	ng/ul#	93
92) Indeno(1,2,3-cd)pyrene	29.18	276	45866m	1.886	ng/ul	
94) Benzo(g,h,i)perylene	30.43	276	39994m	1.994	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
Data File : BG047368.D
Acq On : 20 Nov 2020 1:26
Operator : CG/JU
Sample : L4710-19
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0AW5

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:01 PM

Quant Time: Nov 20 07:38:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 19 14:25:26 2020
Response via : Initial Calibration

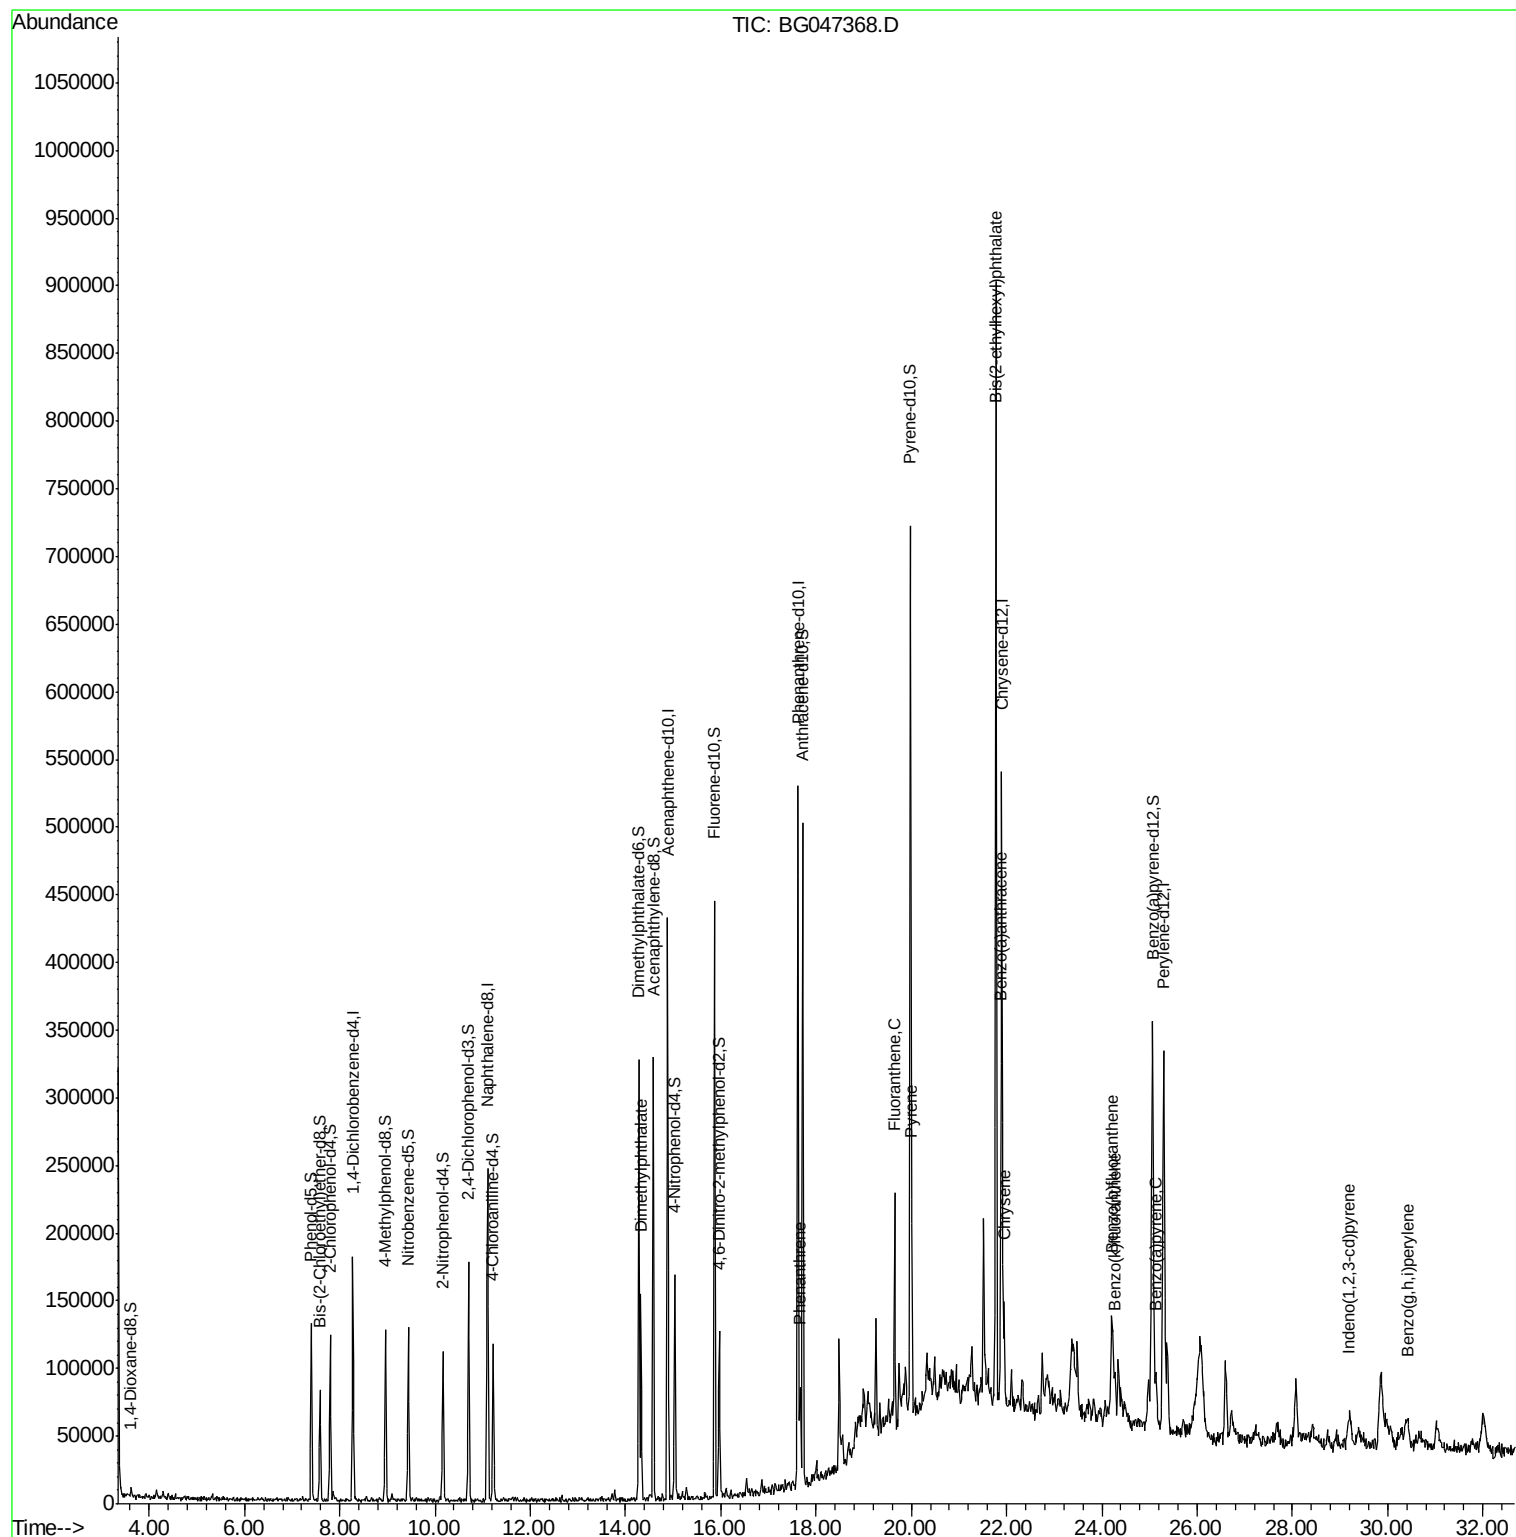

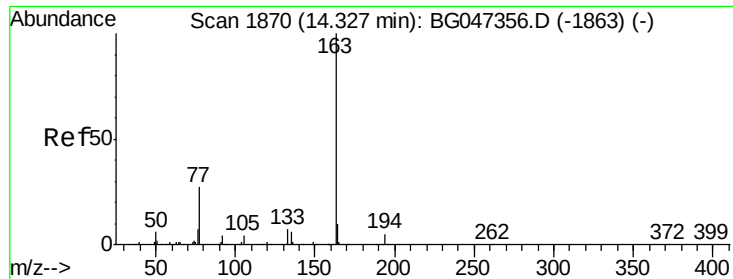





#45
Dimethylphthalate
Concen: 7.104 ng/ul
RT: 14.32 min Scan# 1869
Delta R.T. -0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Instrument :
BNA_G
ClientSampleId :
C0AW5

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.4	3.4	5.2#
164	9.4	8.8	13.2




Manual Integrations
APPROVED


mohammad
11/23/2020 1:29:01 PM

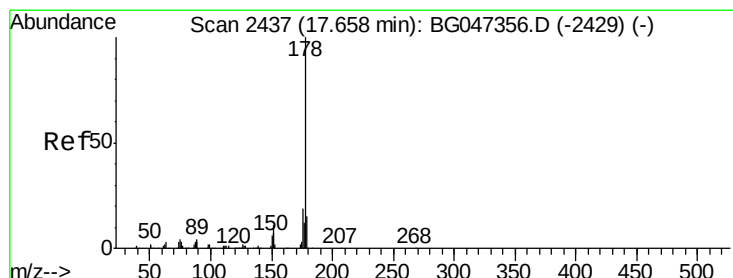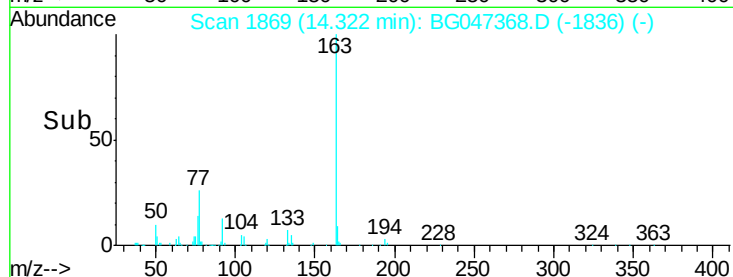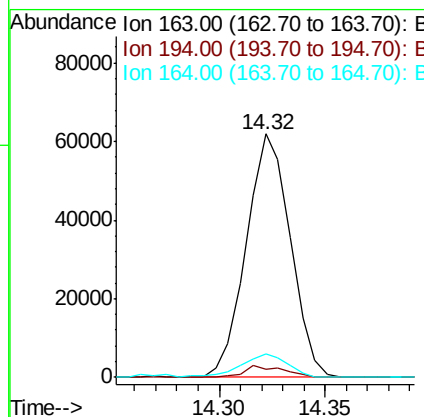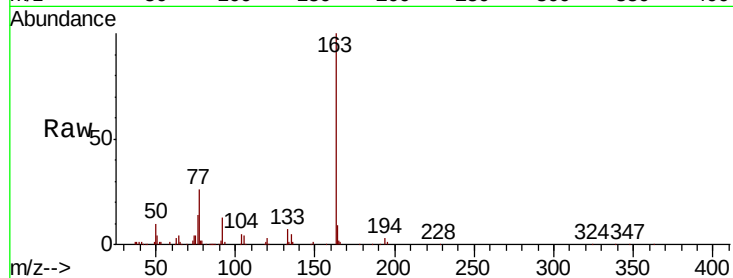

#70
Phenanthrene
Concen: 2.491 ng/ul
RT: 17.66 min Scan# 2437
Delta R.T. 0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.1	12.8	19.2
176	19.8	15.7	23.5

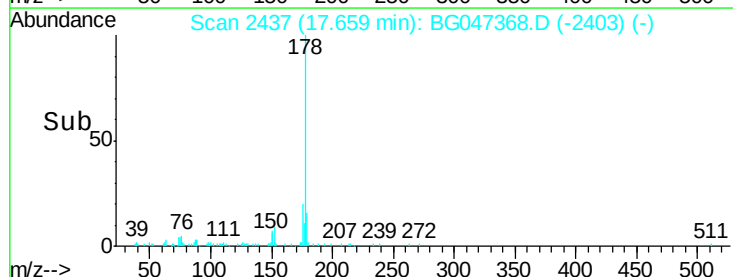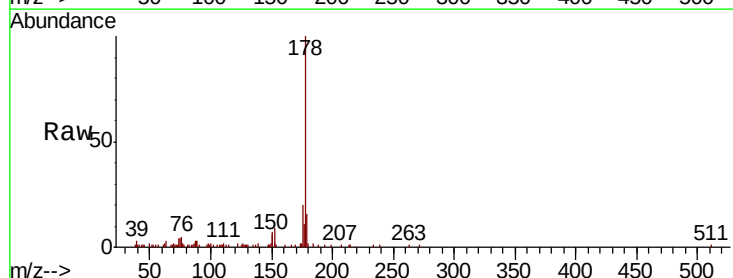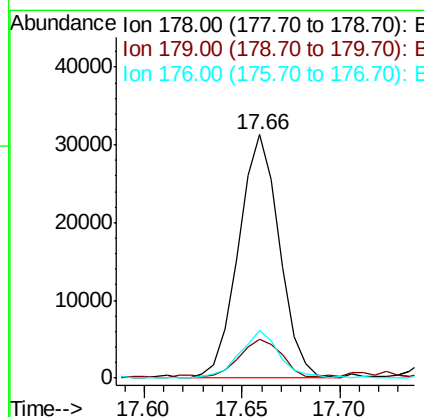

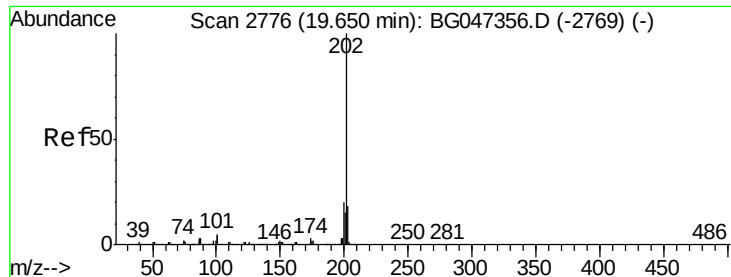





#77
 Fluoranthene
 Concen: 4.807 ng/ul
 RT: 19.65 min Scan# 2776
 Delta R.T. 0.00 min
 Lab File: BG047368.D
 Acq: 20 Nov 2020 1:26

Instrument :
 BNA_G
 ClientSampled :
 C0AW5

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	3.8	3.3	4.9
100	3.0	3.4	5.0#




Manual Integrations
 APPROVED


mohammad
 11/23/2020 1:29:01 PM

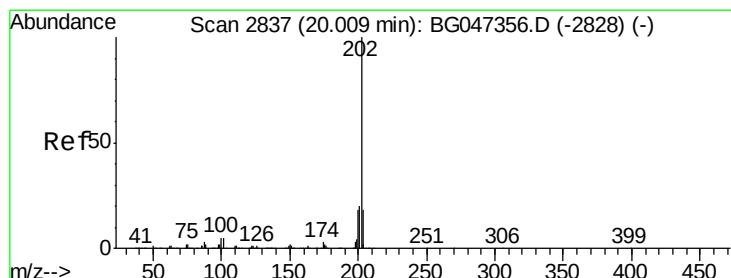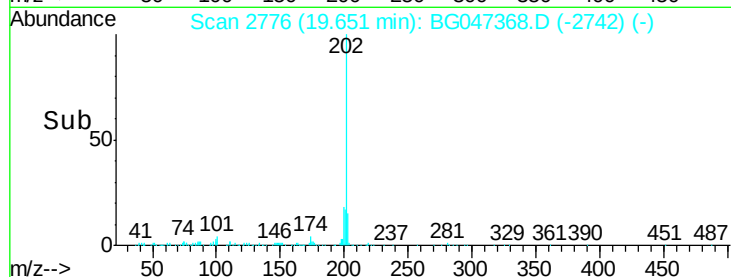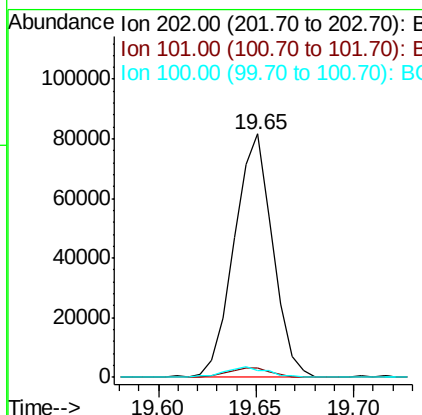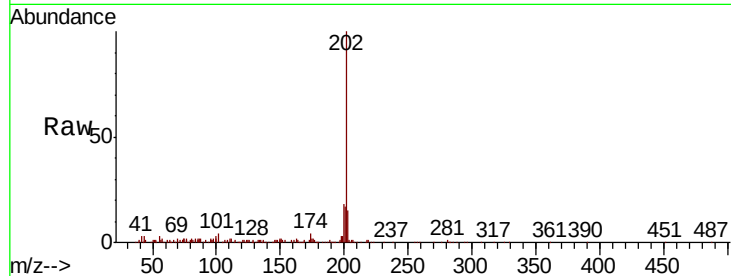

#80
 Pyrene
 Concen: 4.365 ng/ul
 RT: 20.01 min Scan# 2837
 Delta R.T. 0.00 min
 Lab File: BG047368.D
 Acq: 20 Nov 2020 1:26

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	5.7	5.0	7.4
100	4.8	4.6	7.0

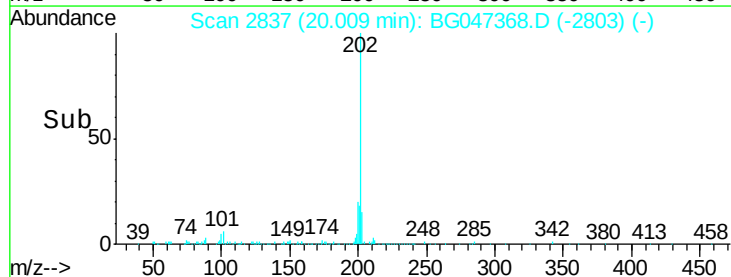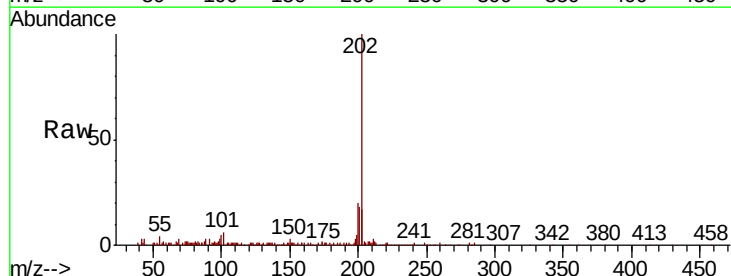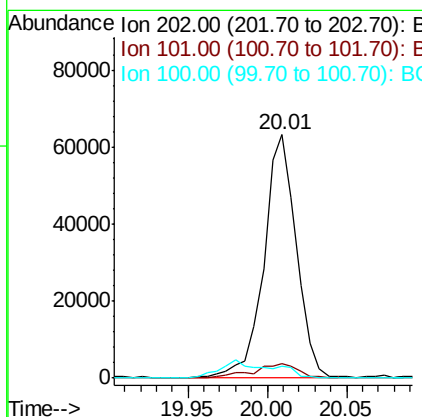

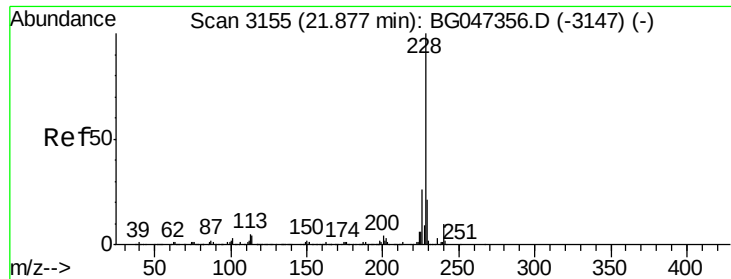





#83
Benzo(a)anthracene
Concen: 2.287 ng/ul
RT: 21.88 min Scan# 3155
Delta R.T. -0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Instrument :
BNA_G
ClientSampleId :
C0AW5

Tot Ion:228	Resp:	47513
Ion Ratio	Lower	Upper
228 100		
229 18.5	16.2	24.2
226 24.5	23.3	34.9




Manual Integrations
APPROVED


mohammad
11/23/2020 1:29:01 PM

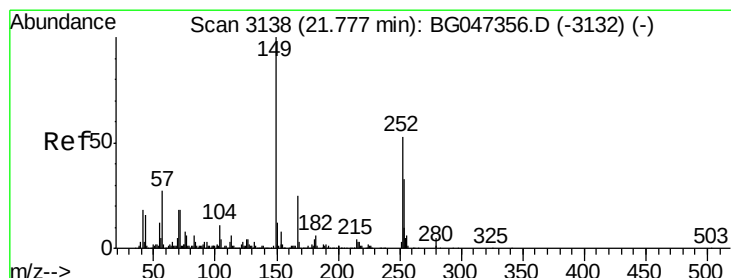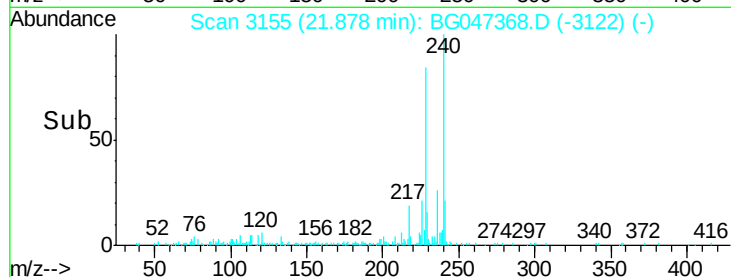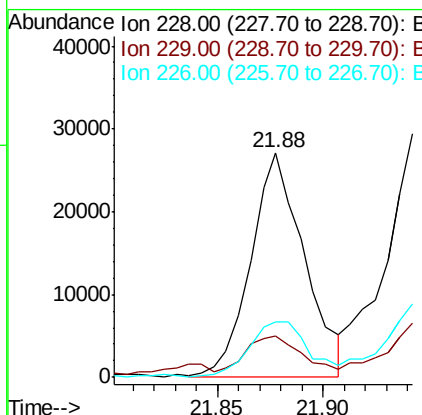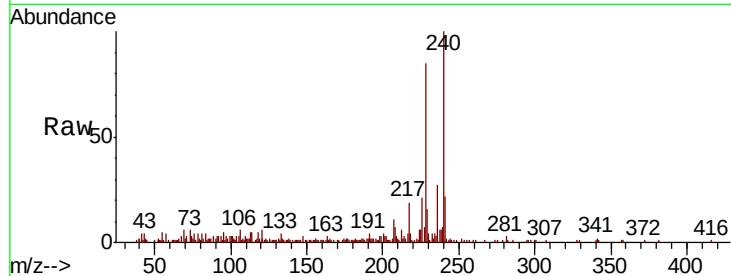

#84
Bis(2-ethylhexyl)phthalate
Concen: 32.308 ng/ul
RT: 21.78 min Scan# 3138
Delta R.T. 0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Tgt Ion:149	Resp:	327111
Ion Ratio	Lower	Upper
149 100		
167 28.3	21.8	32.8
279 6.0	4.2	6.2

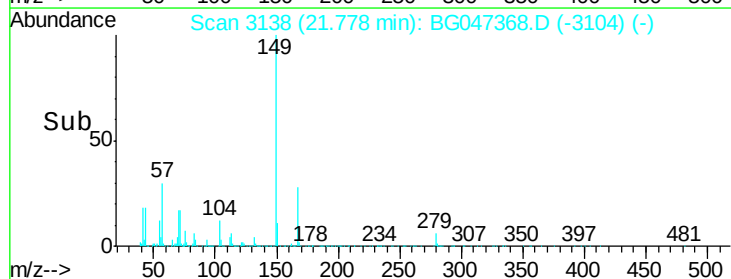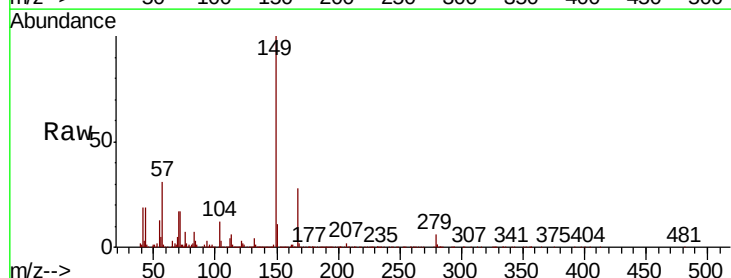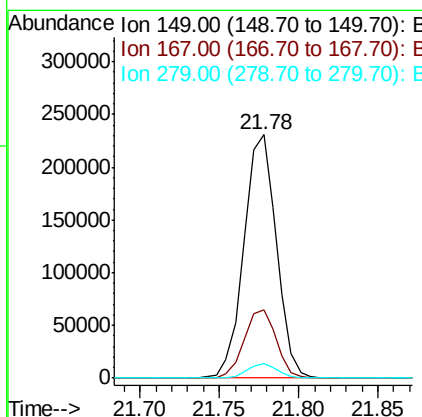

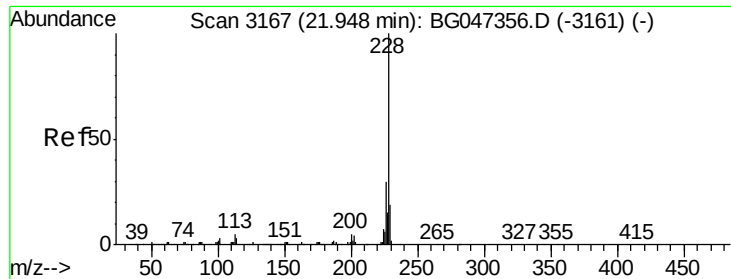





#85
Chrysene
Concen: 2.828 ng/ul
RT: 21.94 min Scan# 3166
Delta R.T. -0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Instrument :
BNA_G
ClientSampleId :
C0AW5

Tot Ion	Ion	Ratio	Resp	Lower	Upper
228	100		55910		
226	30.3		23.8	35.6	
229	22.0		16.3	24.5	




Manual Integrations
APPROVED


mohammad
11/23/2020 1:29:01 PM

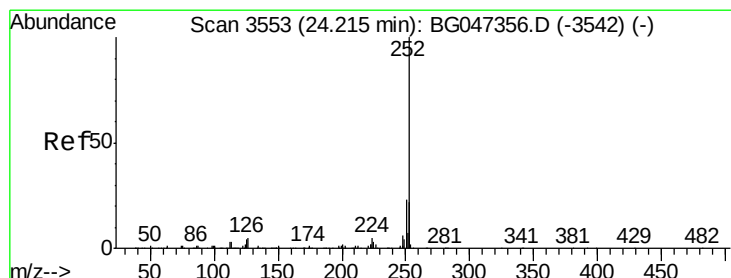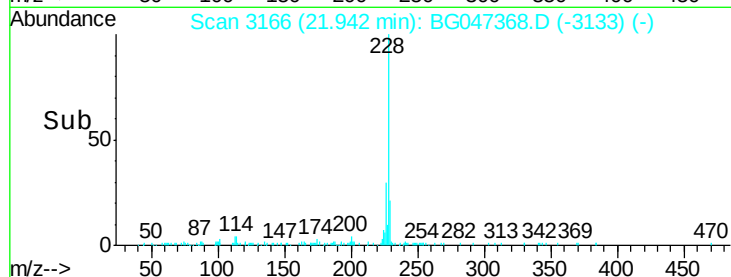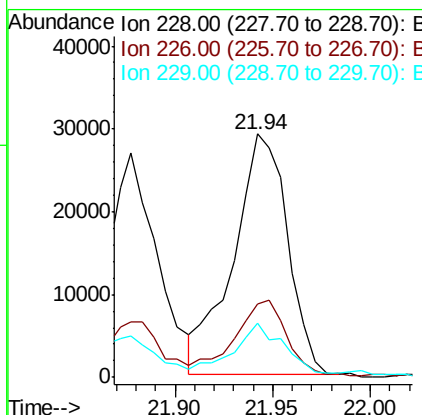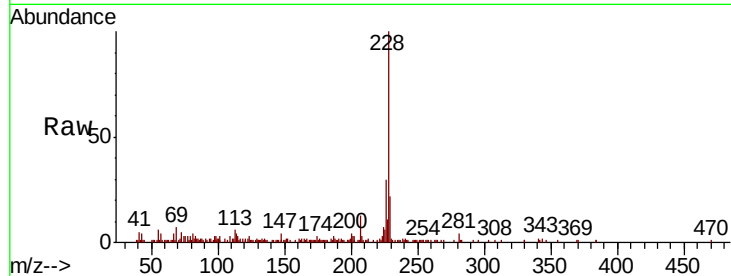

#88
Benzo(b)fluoranthene
Concen: 3.715 ng/ul m
RT: 24.21 min Scan# 3552
Delta R.T. 0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
252	100		83293		
253	21.5		18.4	27.6	
125	4.5		2.5	3.7#	

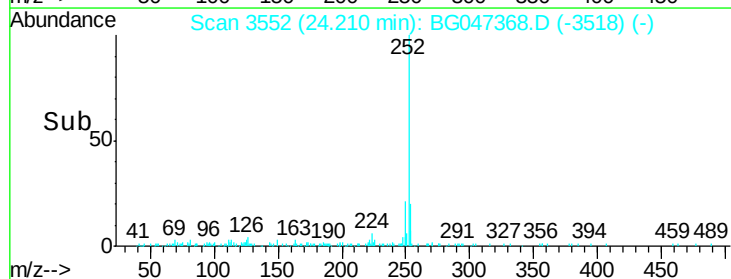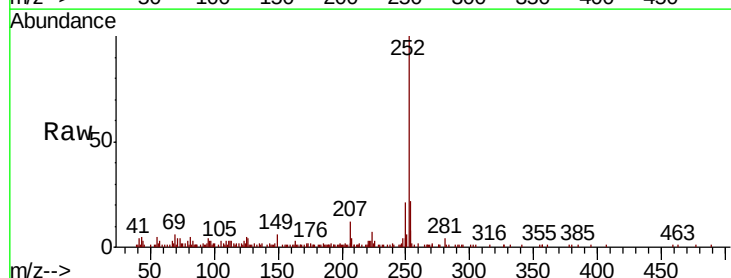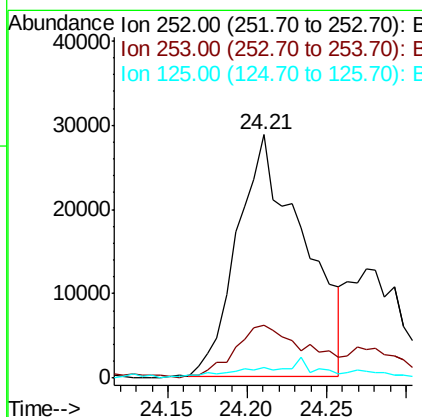

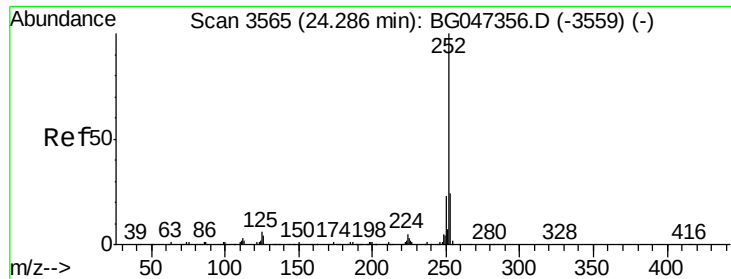





#89
Benzo(k)fluoranthene
Concen: 1.327 ng/ul m
RT: 24.27 min Scan# 3563
Delta R.T. -0.01 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Instrument :
BNA_G
ClientSampled :
C0AW5

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.8	16.7	25.1#
125	5.8	2.6	3.8#




Manual Integrations
APPROVED


mohammad
11/23/2020 1:29:01 PM

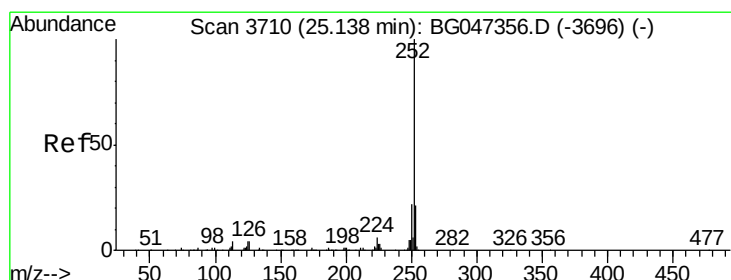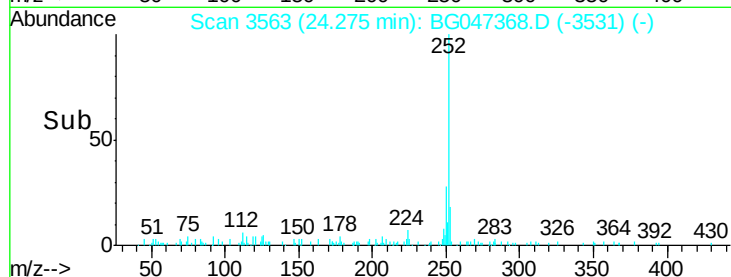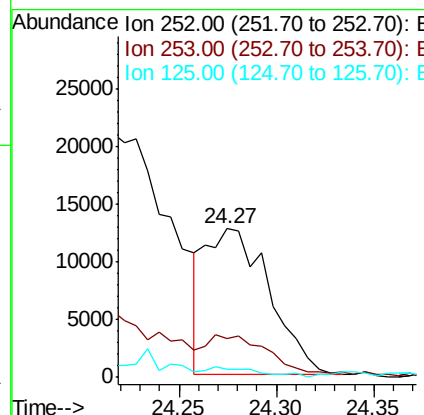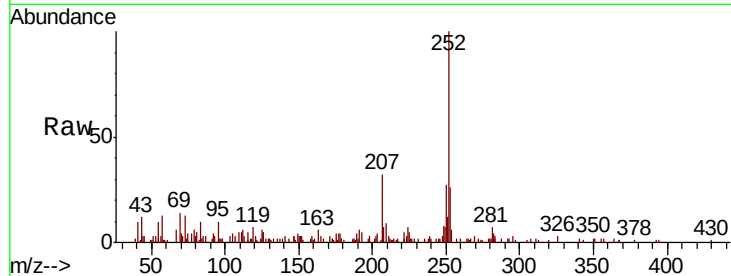

#91
Benzo(a)pyrene
Concen: 2.755 ng/ul
RT: 25.14 min Scan# 3710
Delta R.T. 0.00 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.6	17.5	26.3
125	8.8	3.1	4.7#

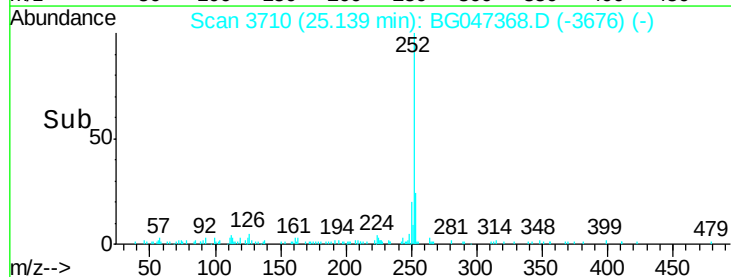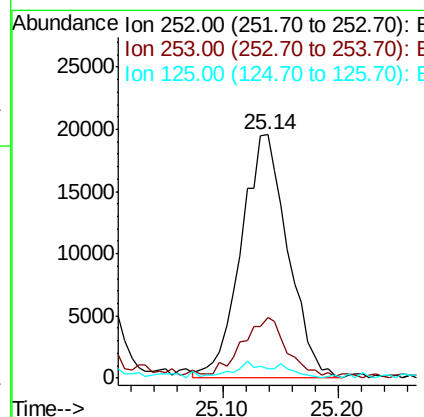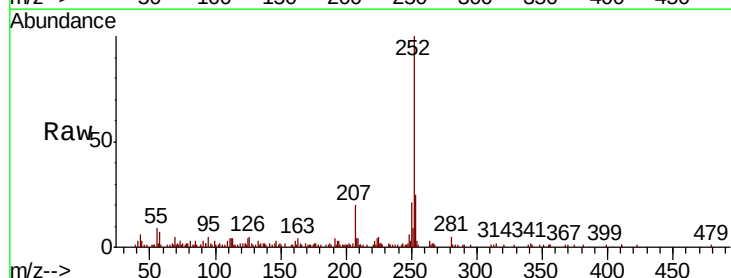

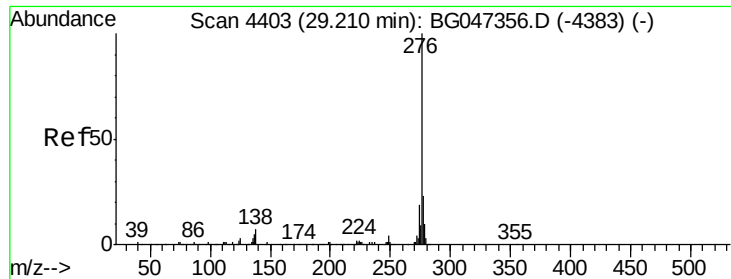

#92





Indeno(1,2,3-cd)pyrene
Concen: 1.886 ng/ul m
RT: 29.18 min Scan# 4398
Delta R.T. -0.02 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Instrument :
BNA_G
ClientSampleId :
C0AW5

Tot Ion	Ratio	Lower	Upper
276	100		
138	14.3	7.5	11.3#
277	26.7	19.9	29.9

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:01 PM

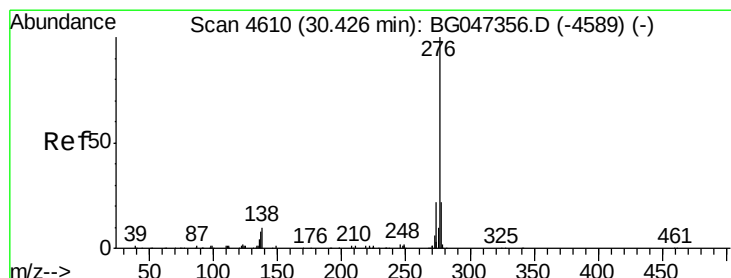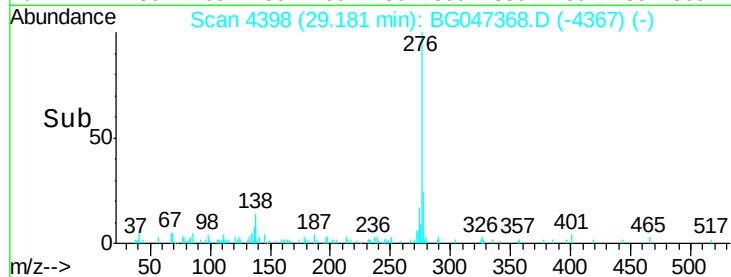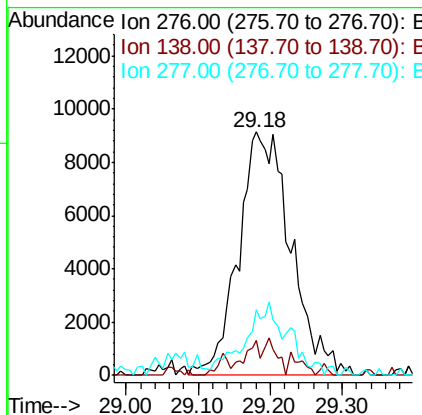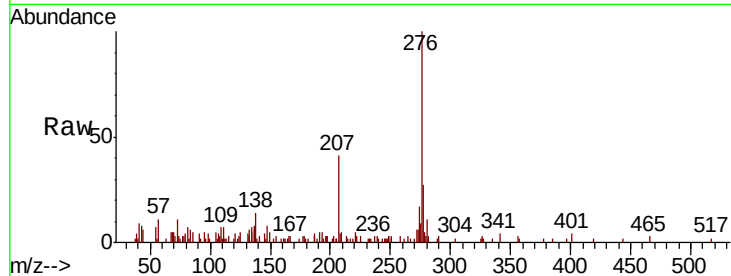

#94

Benzo(g,h,i)perylene
Concen: 1.994 ng/ul m
RT: 30.43 min Scan# 4610
Delta R.T. 0.01 min
Lab File: BG047368.D
Acq: 20 Nov 2020 1:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	10.3	8.2	12.2
277	16.3	17.5	26.3#

