

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
 Data File : BG047375.D
 Acq On : 20 Nov 2020 10:43
 Operator : CG/JU
 Sample : L4794-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BH0

Quant Time: Nov 20 11:52:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 19 14:25:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	35284	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	146922	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	105618	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.61	188	274732	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	257398	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	264940	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.61	96	4459	4.59	ng/uL	0.00
5) Phenol-d5	7.40	99	19878	5.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	52538	26.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	52966	22.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	38430	14.13	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	34577	28.49	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	36445	27.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	75977	25.06	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	6144	2.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	284536	31.38	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	323497	30.87	ng/ul	0.00
52) 4-Nitrophenol-d4	15.04	143	9010	6.51	ng/ul	0.00
58) Fluorene-d10	15.87	176	262979	31.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	45298	28.97	ng/ul	0.00
71) Anthracene-d10	17.71	188	450508	33.06	ng/ul	0.00
79) Pyrene-d10	19.98	212	507275	33.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	502471	32.95	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	14.32	163	21309	2.304 ng/ul# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
Data File : BG047375.D
Acq On : 20 Nov 2020 10:43
Operator : CG/JU
Sample : L4794-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BH0

Quant Time: Nov 20 11:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 19 14:25:26 2020
Response via : Initial Calibration

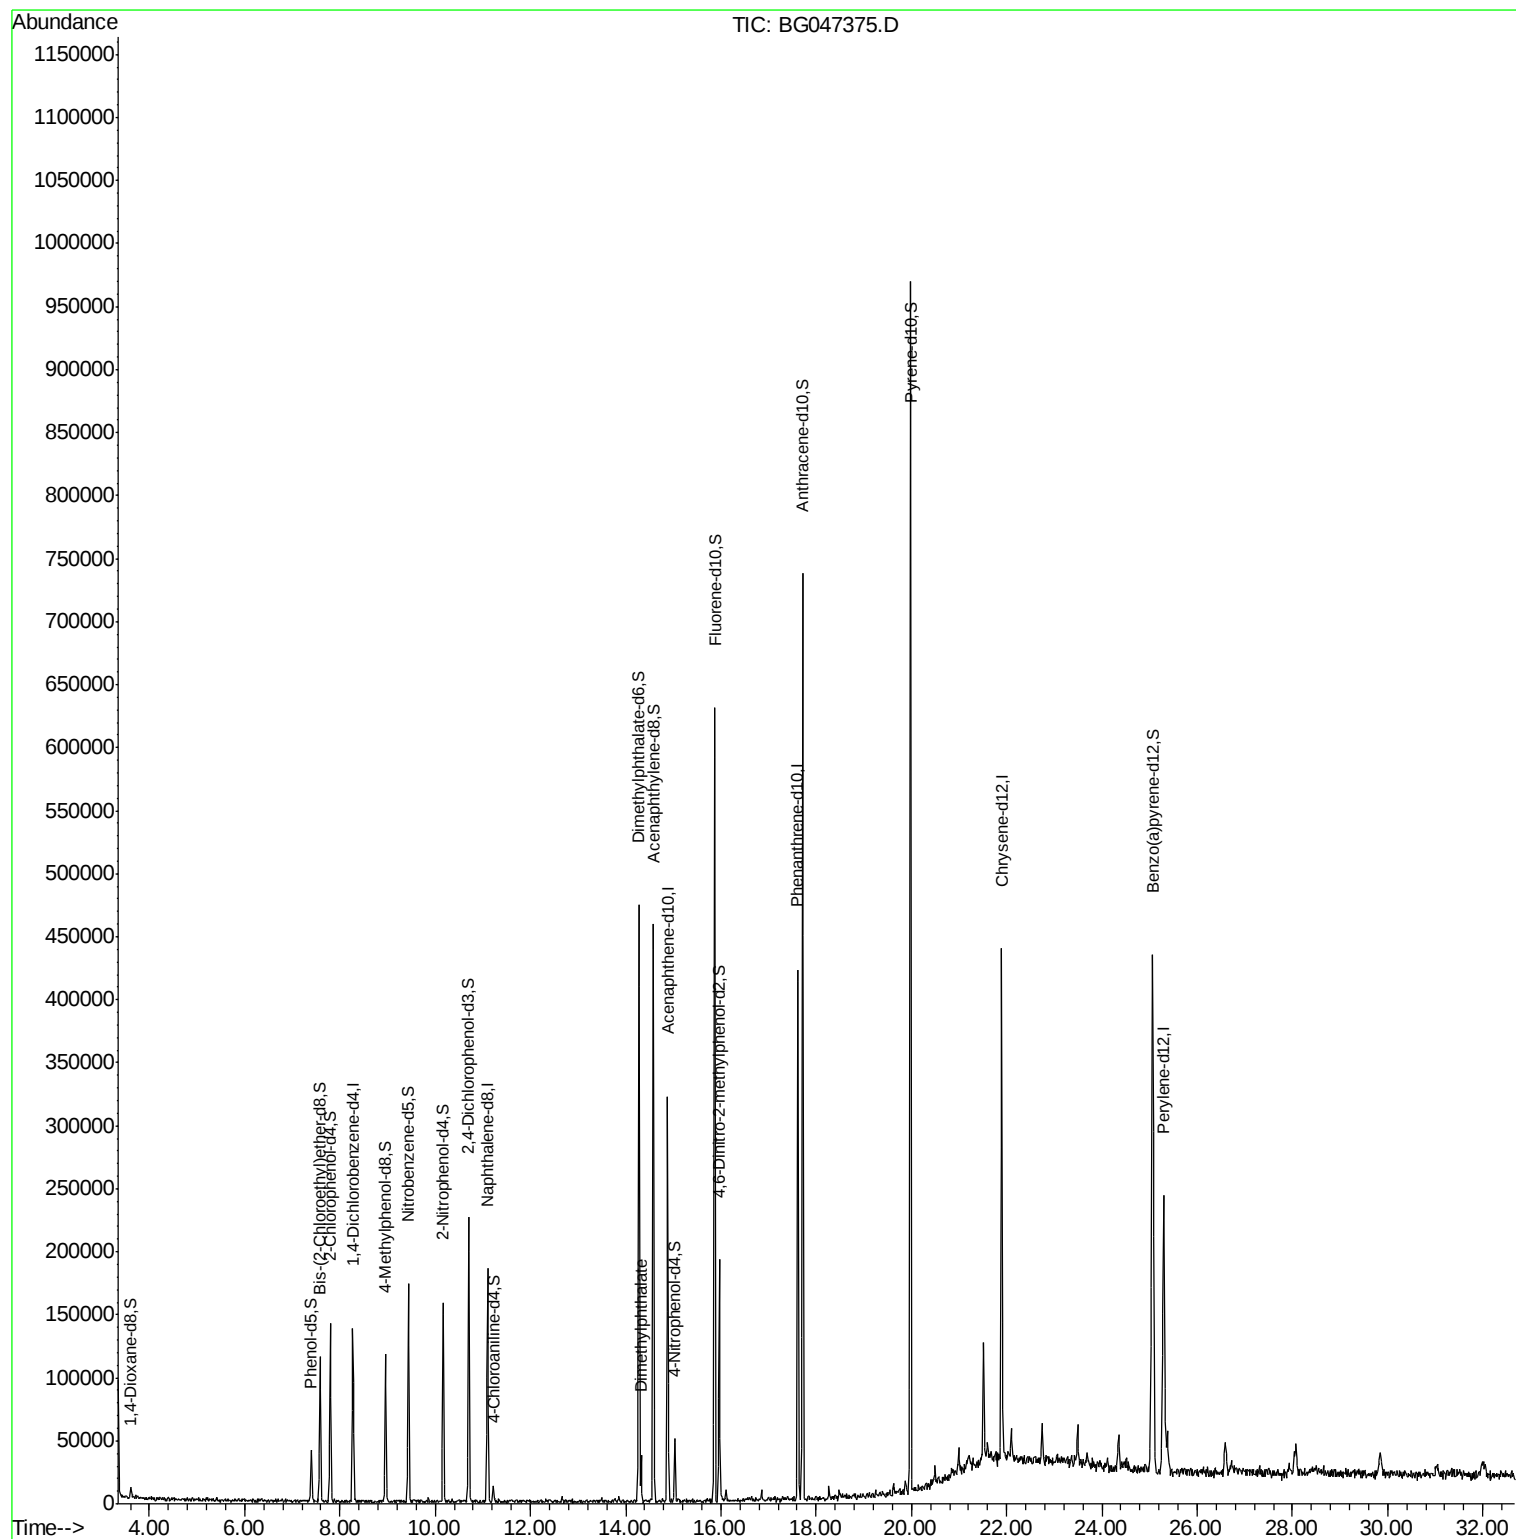

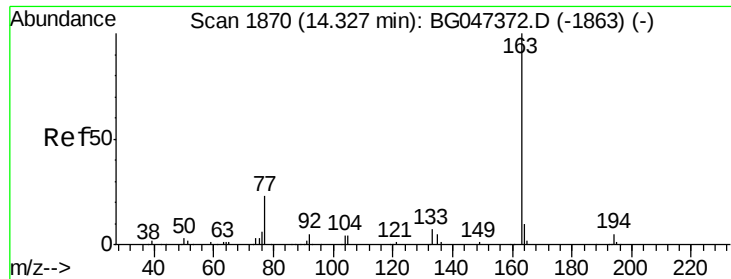

#45

Dimethylphthalate

Concen: 2.304 ng/ul

RT: 14.32 min Scan# 1870

Delta R.T. -0.00 min

Lab File: BG047375.D

Acq: 20 Nov 2020 10:43

Instrument :

BNA_G

ClientSampleId :

C0BH0

Tot Ion:163 Resp: 21309

Ion Ratio Lower Upper

163 100

194 6.9 3.4 5.2#

164 9.1 8.8 13.2

