

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
 Data File : BG047371.D
 Acq On : 20 Nov 2020 3:27
 Operator : CG/JU
 Sample : L4748-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.890	92	94	96	rBV3	3382	1988	0.26%	0.071%
2	3.996	110	112	115	rBV3	3567	2864	0.38%	0.102%
3	4.518	199	201	202	rBV2	3547	2343	0.31%	0.083%
4	4.865	258	260	262	rBV3	3617	2529	0.33%	0.090%
5	5.030	286	288	291	rVB	2870	2929	0.38%	0.104%
6	5.488	364	366	369	rVB	2320	1952	0.26%	0.069%
7	5.987	447	451	452	rBV2	1944	2458	0.32%	0.087%
8	6.152	474	479	481	rBV	2999	4375	0.57%	0.155%
9	6.604	552	556	560	rVB3	1698	2678	0.35%	0.095%
10	6.657	563	565	567	rBV3	1505	1854	0.24%	0.066%
11	6.781	584	586	588	rBV2	2655	2303	0.30%	0.082%
12	6.886	602	604	607	rBV	2568	2662	0.35%	0.095%
13	7.162	650	651	654	rBV	2914	2766	0.36%	0.098%
14	7.280	670	671	675	rVB3	2747	2696	0.35%	0.096%
15	7.345	680	682	684	rBV	2078	2015	0.26%	0.072%
16	7.421	692	695	698	rBV	1880	2067	0.27%	0.073%
17	7.621	728	729	732	rBV	2481	2504	0.33%	0.089%
18	7.938	781	783	787	rVB2	3696	2712	0.36%	0.096%
19	8.273	834	840	848	rVB	150344	263744	34.59%	9.373%
20	8.402	859	862	865	rBV2	1376	1870	0.25%	0.066%
21	8.479	872	875	879	rBV	2453	4031	0.53%	0.143%
22	8.766	921	924	927	rVB2	2567	2610	0.34%	0.093%
23	8.843	935	937	940	rVB	2519	2198	0.29%	0.078%
24	9.236	1001	1004	1007	rBV	2118	3383	0.44%	0.120%
25	9.454	1038	1041	1043	rBV	1644	1947	0.26%	0.069%
26	9.795	1094	1099	1102	rBV2	1623	2716	0.36%	0.097%
27	10.012	1133	1136	1138	rBV2	1881	2244	0.29%	0.080%
28	10.476	1214	1215	1220	rBV	1958	2260	0.30%	0.080%
29	10.870	1281	1282	1286	rVB	1893	2222	0.29%	0.079%
30	11.099	1315	1321	1330	rVB	195405	368959	48.39%	13.112%
31	11.205	1335	1339	1341	rBV	1453	2327	0.31%	0.083%
32	11.463	1381	1383	1385	rBV2	1951	1828	0.24%	0.065%
33	11.716	1424	1426	1428	rBV	2455	1917	0.25%	0.068%
34	11.851	1447	1449	1451	rBV	1752	1838	0.24%	0.065%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
 Data File : BG047371.D
 Acq On : 20 Nov 2020 3:27
 Operator : CG/JU
 Sample : L4748-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	11.974	1467	1470	1472	rBV	2080	2728	0.36%	0.097%
36	12.891	1623	1626	1628	rBV	1949	2156	0.28%	0.077%
37	13.173	1671	1674	1676	rBV	2034	2154	0.28%	0.077%
38	13.343	1699	1703	1705	rBV	2042	1840	0.24%	0.065%
39	14.166	1838	1843	1844	rVB	1713	2491	0.33%	0.089%
40	14.178	1844	1845	1847	rBV	2367	1901	0.25%	0.068%
41	14.331	1869	1871	1875	rVB	2508	2016	0.26%	0.072%
42	14.372	1875	1878	1882	rVB2	2536	2432	0.32%	0.086%
43	14.648	1922	1925	1927	rBV	1683	2444	0.32%	0.087%
44	14.883	1958	1965	1972	rBV2	342321	556218	72.95%	19.767%
45	15.229	2023	2024	2027	rBV	2469	2205	0.29%	0.078%
46	15.323	2038	2040	2044	rVB	1787	1803	0.24%	0.064%
47	16.005	2153	2156	2158	rBV	1354	1909	0.25%	0.068%
48	16.211	2189	2191	2195	rVB	1788	2208	0.29%	0.078%
49	16.258	2195	2199	2201	rBV	1862	2880	0.38%	0.102%
50	16.358	2214	2216	2218	rBV	2006	2396	0.31%	0.085%
51	16.587	2252	2255	2257	rBV	1846	1971	0.26%	0.070%
52	17.063	2334	2336	2340	rBV	1930	2332	0.31%	0.083%
53	17.145	2349	2350	2352	rBV	2575	2054	0.27%	0.073%
54	17.168	2352	2354	2355	rVB2	3350	2248	0.29%	0.080%
55	17.362	2385	2387	2390	rBV	1630	2398	0.31%	0.085%
56	17.409	2390	2395	2397	rVV3	3983	5566	0.73%	0.198%
57	17.433	2397	2399	2402	rVB3	2581	2517	0.33%	0.089%
58	17.615	2423	2430	2436	rBV	467830	723957	94.95%	25.729%
59	17.668	2436	2439	2441	rBV	2305	1932	0.25%	0.069%
60	18.073	2506	2508	2514	rVB2	2391	2797	0.37%	0.099%
61	18.279	2541	2543	2544	rBV	2618	2040	0.27%	0.072%
62	21.898	3153	3159	3167	rVB2	448835	762426	100.00%	27.096%


Sum of corrected areas: 2813808

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111920\
Data File : BG047371.D
Acq On : 20 Nov 2020 3:27
Operator : CG/JU
Sample : L4748-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

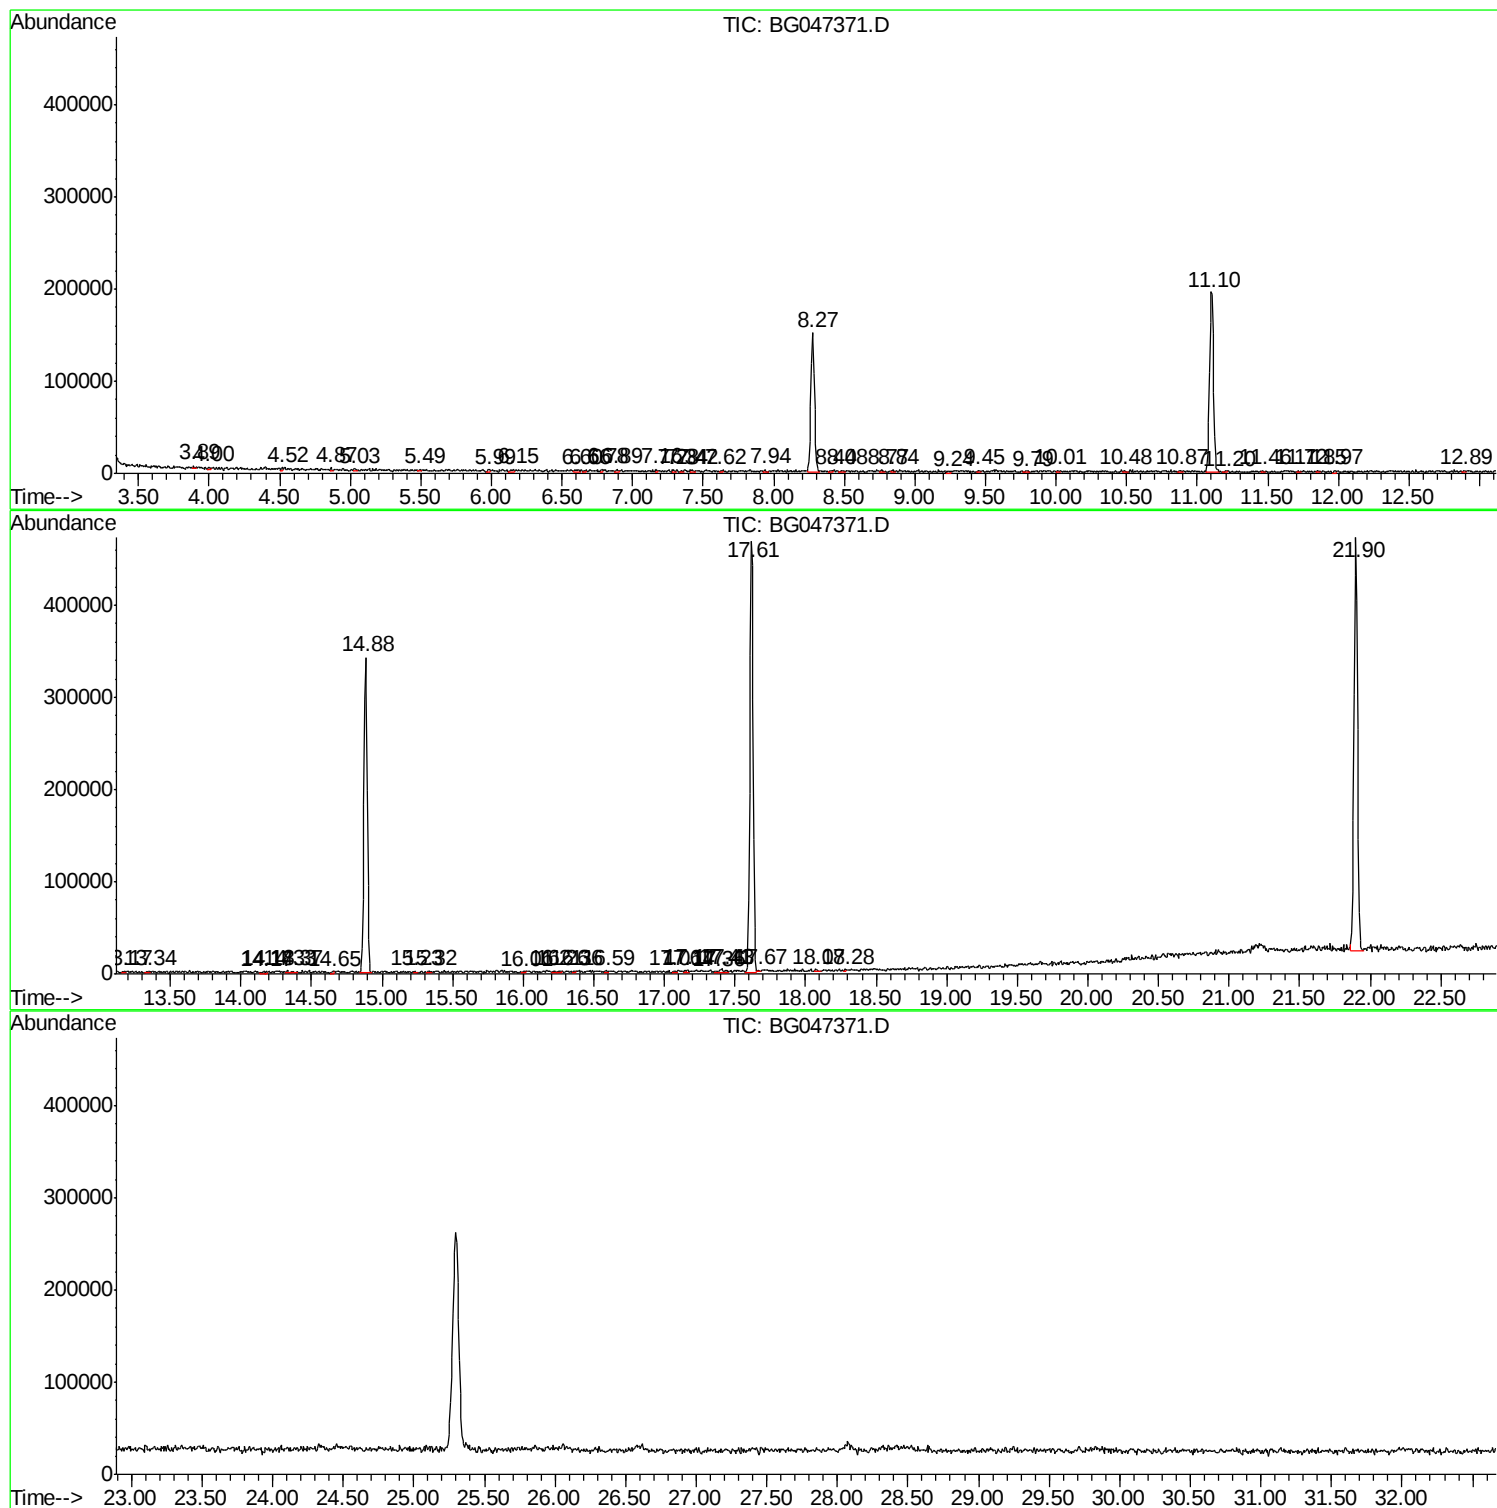

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG111920\
Data_File : BG047371.D
Acq_On : 20 Nov 2020 3:27
Operator : CG/JUU
Sample : L4748-100
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SVOC-GCP2-BLANK

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
