
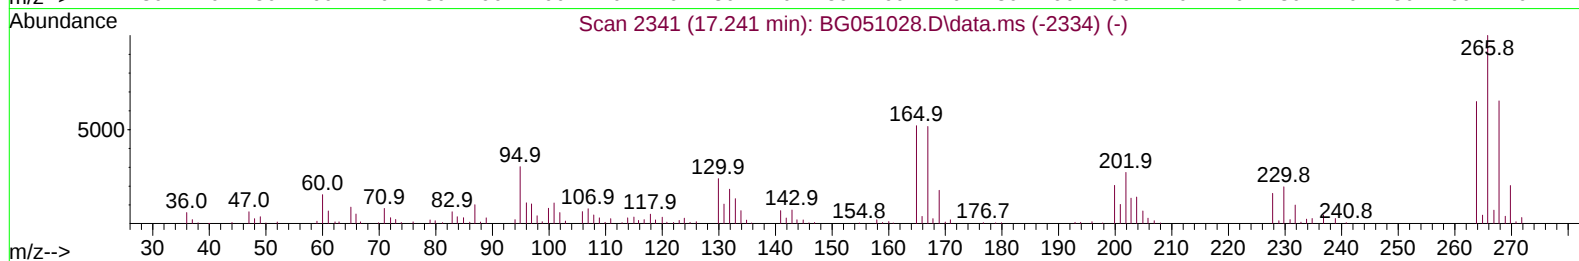
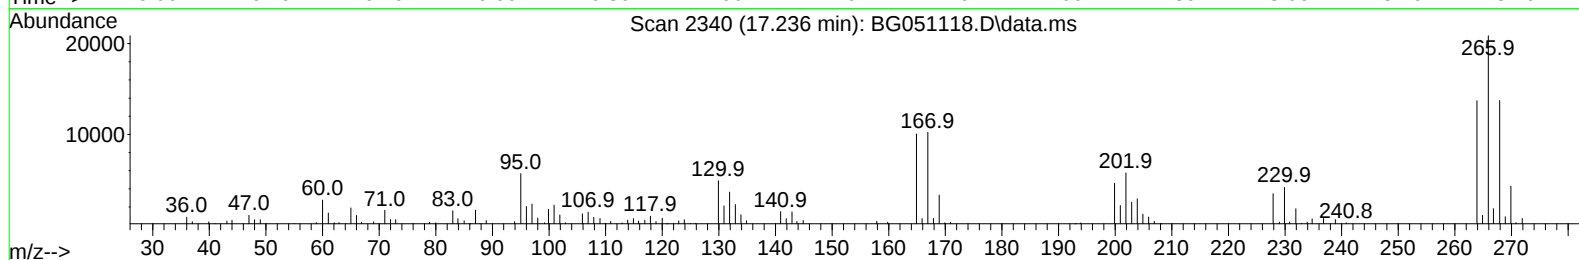


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051118.D
Acq On : 19 Nov 2021 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 11:52:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:48:56 2021
Response via : Initial Calibration

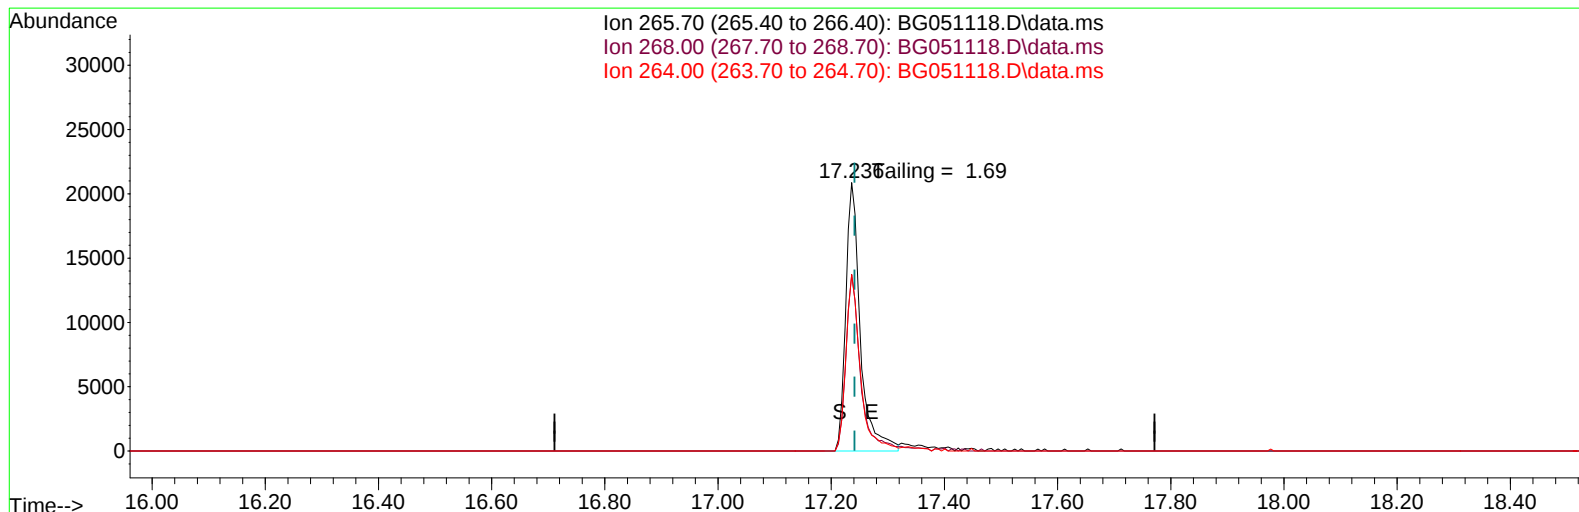

TIC: BG051118.D\data.ms

(70) Pentachlorophenol (C)




17.236min (-0.005) 4732.60 ng

response 37355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.76
264.00	61.30	65.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051118.D
Acq On : 19 Nov 2021 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 11:52:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:48:56 2021
Response via : Initial Calibration

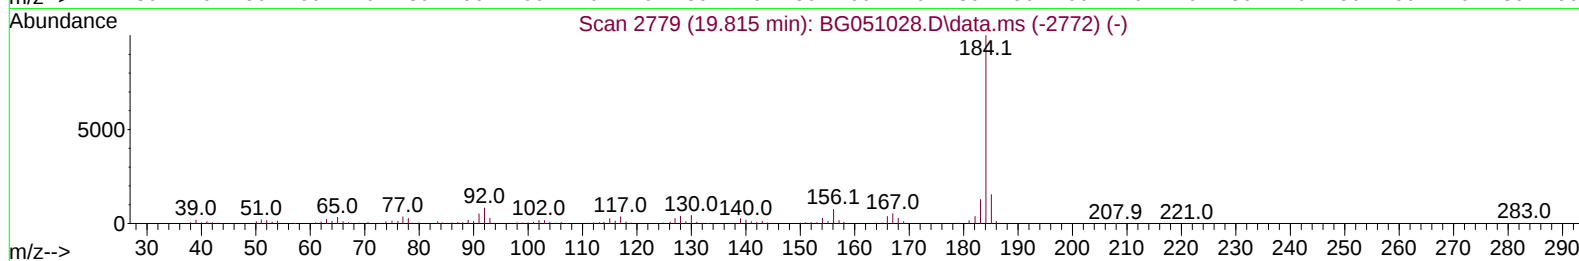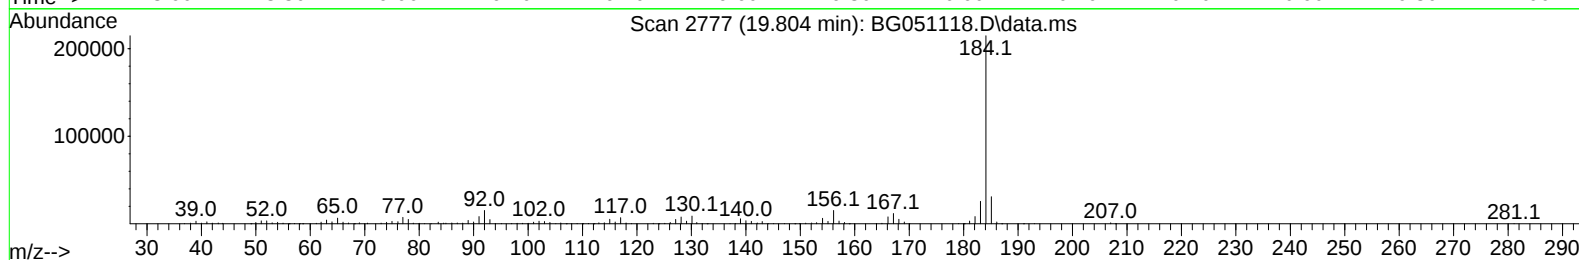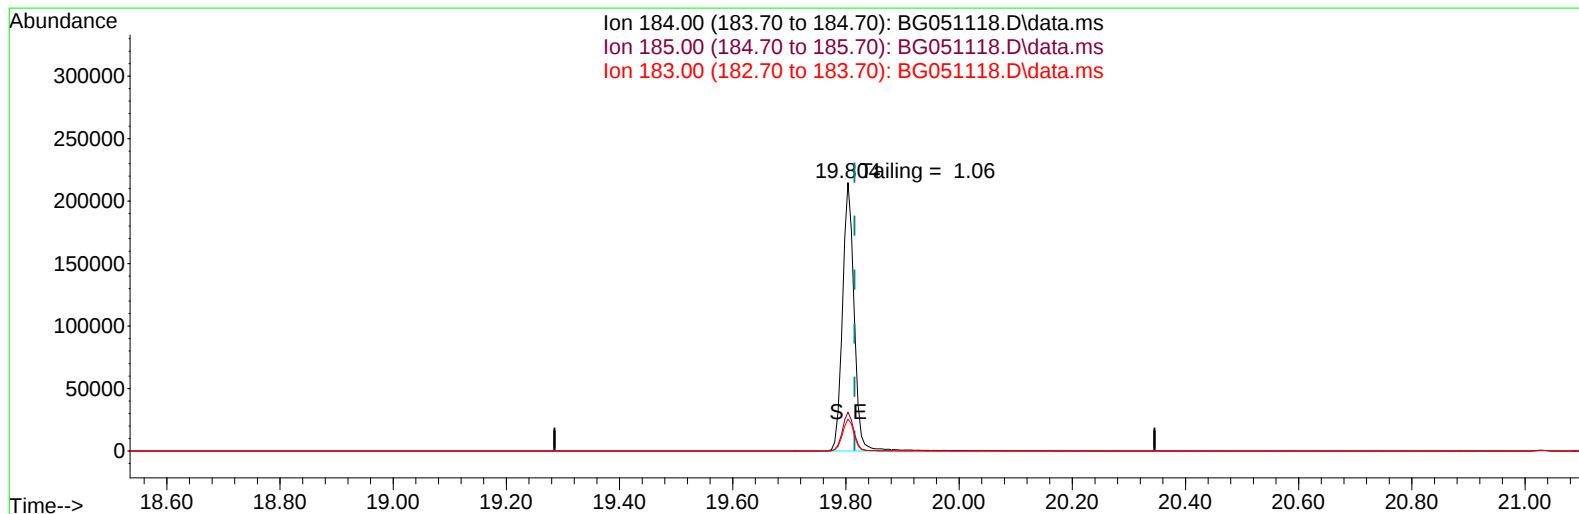

TIC: BG051118.D\data.ms

(77) Benzidine

19.804min (-0.011) 0.00 ng

response 306174

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.48
183.00	11.70	11.96
0.00	0.00	0.00