
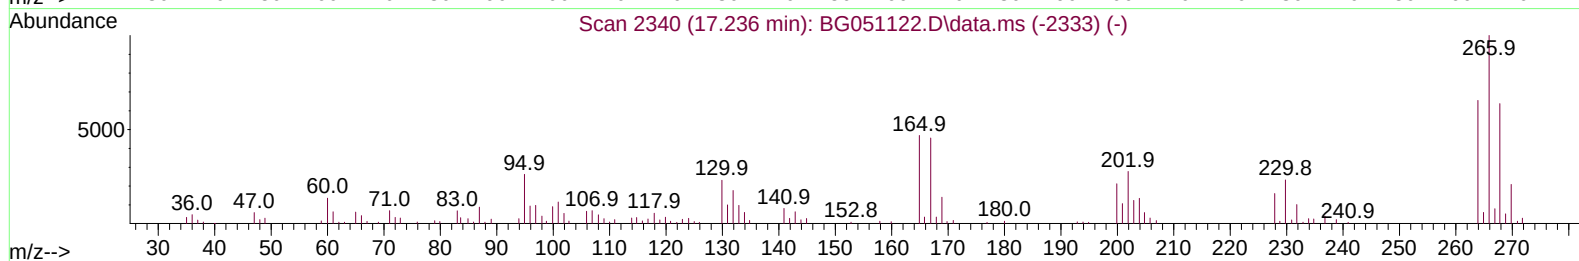
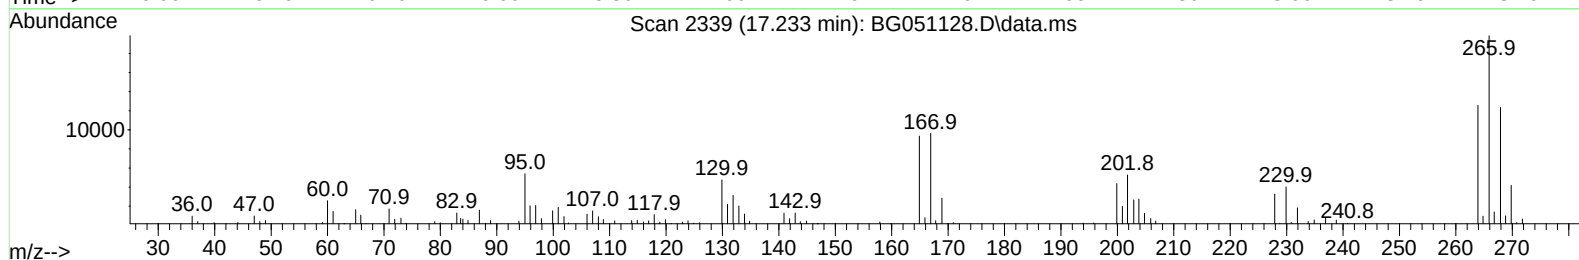


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051128.D
Acq On : 19 Nov 2021 18:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 19:10:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

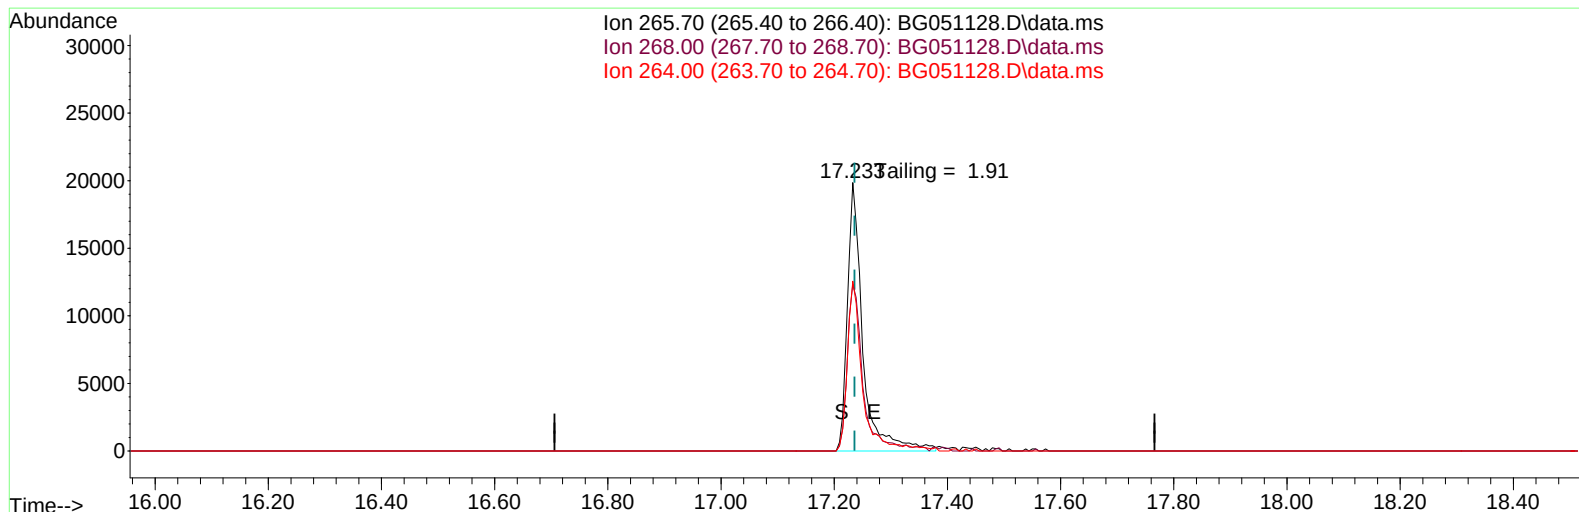

TIC: BG051128.D\data.ms

(70) Pentachlorophenol (C)




17.233min (-0.003) 27828.96 ng

response 36995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.18
264.00	61.30	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051128.D
Acq On : 19 Nov 2021 18:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 19:10:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

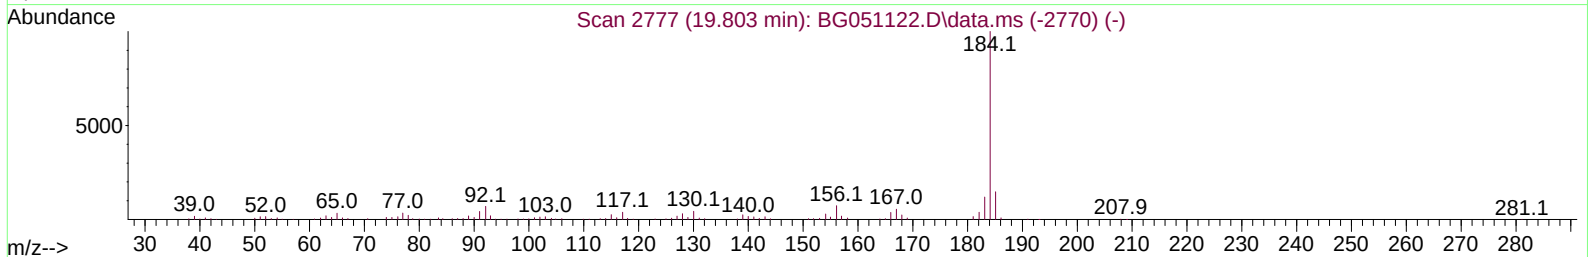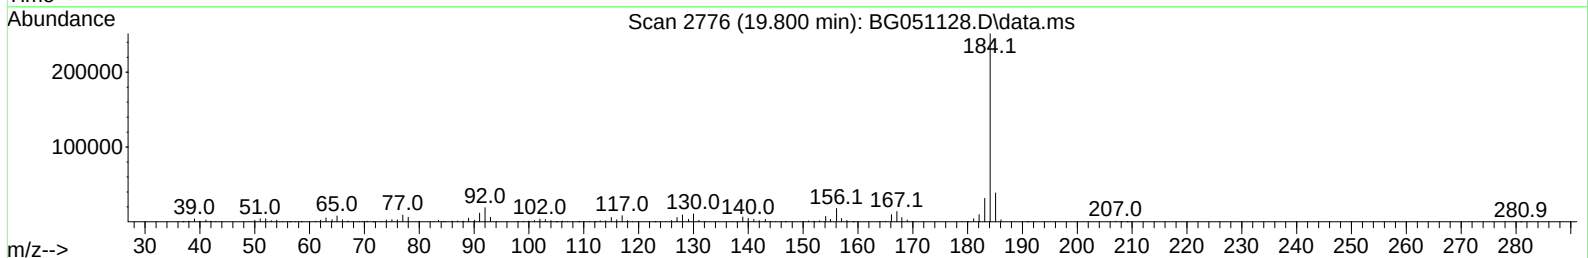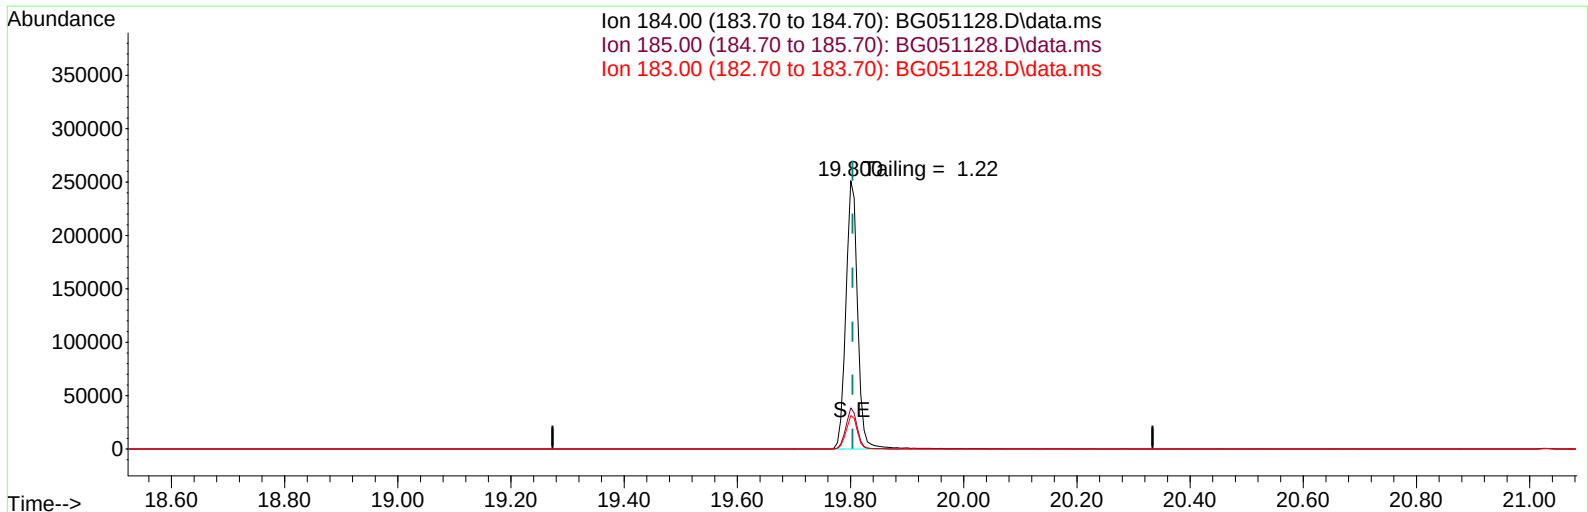

TIC: BG051128.D\data.ms

(77) Benzidine

19.800min (-0.003) 0.00 ng

response 358393

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.36
183.00	11.70	12.48
0.00	0.00	0.00