

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
 Data File : BG051130.D  
 Acq On : 19 Nov 2021 19:57  
 Operator : CG/JU  
 Sample : PB140900BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB140900BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG051130.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.747       | 377           | 384         | 398          | rBV      | 504089         | 823199        | 34.16%          | 9.170%        |
| 2         | 7.363       | 651           | 659         | 677          | rBV      | 497227         | 879098        | 36.47%          | 9.793%        |
| 3         | 8.209       | 795           | 803         | 811          | rVB      | 83459          | 143968        | 5.97%           | 1.604%        |
| 4         | 9.384       | 995           | 1003        | 1015         | rBV      | 298589         | 549649        | 22.81%          | 6.123%        |
| 5         | 11.035      | 1276          | 1284        | 1294         | rBV      | 112302         | 208145        | 8.64%           | 2.319%        |
| 6         | 13.456      | 1689          | 1696        | 1709         | rBV      | 839667         | 1305311       | 54.16%          | 14.541%       |
| 7         | 14.836      | 1924          | 1931        | 1940         | rBV      | 203800         | 321765        | 13.35%          | 3.584%        |
| 8         | 16.323      | 2178          | 2184        | 2199         | rBV      | 618238         | 973728        | 40.40%          | 10.847%       |
| 9         | 17.580      | 2392          | 2398        | 2406         | rBV      | 265077         | 420373        | 17.44%          | 4.683%        |
| 10        | 20.171      | 2833          | 2839        | 2845         | rBV      | 1866309        | 2410178       | 100.00%         | 26.849%       |
| 11        | 21.881      | 3123          | 3130        | 3137         | rVB      | 274183         | 472861        | 19.62%          | 5.268%        |
| 12        | 25.271      | 3697          | 3707        | 3721         | rVB2     | 156308         | 468450        | 19.44%          | 5.218%        |




Sum of corrected areas: 8976725

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
Data File : BG051130.D  
Acq On : 19 Nov 2021 19:57  
Operator : CG/JU  
Sample : PB140900BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140900BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

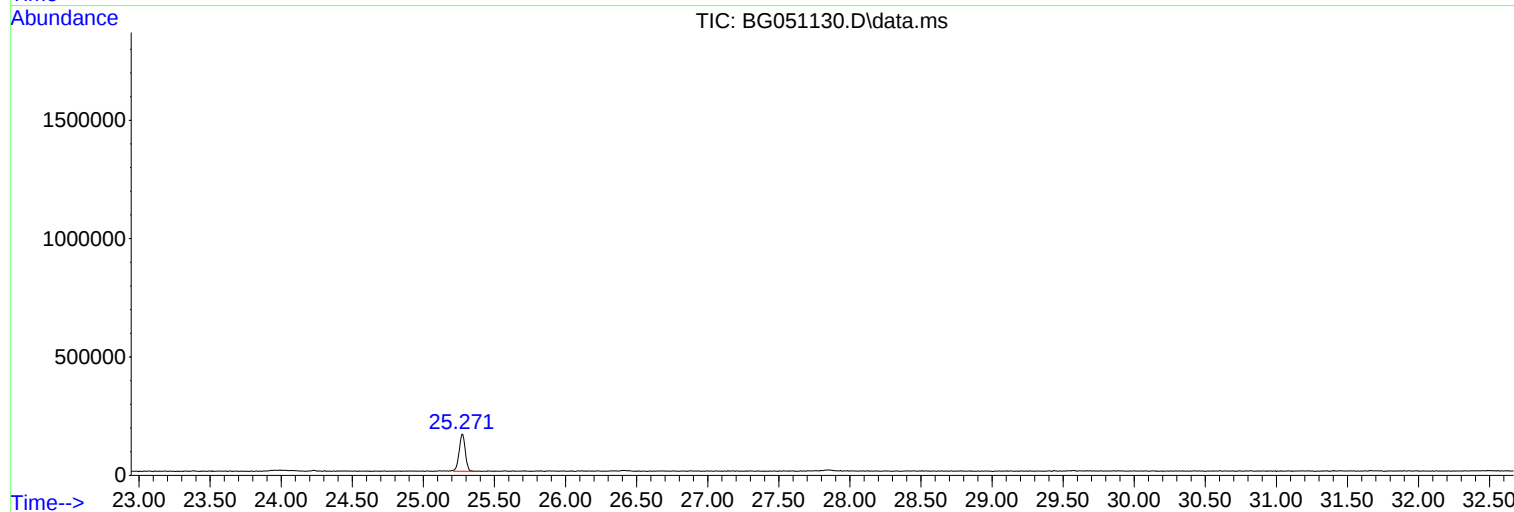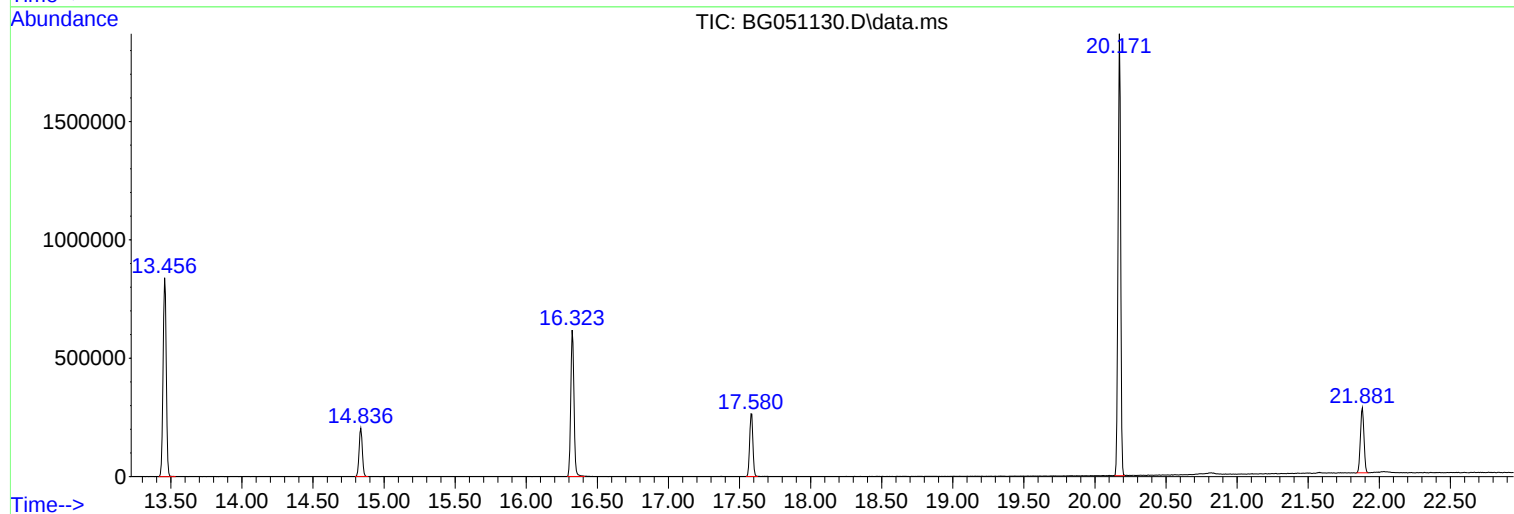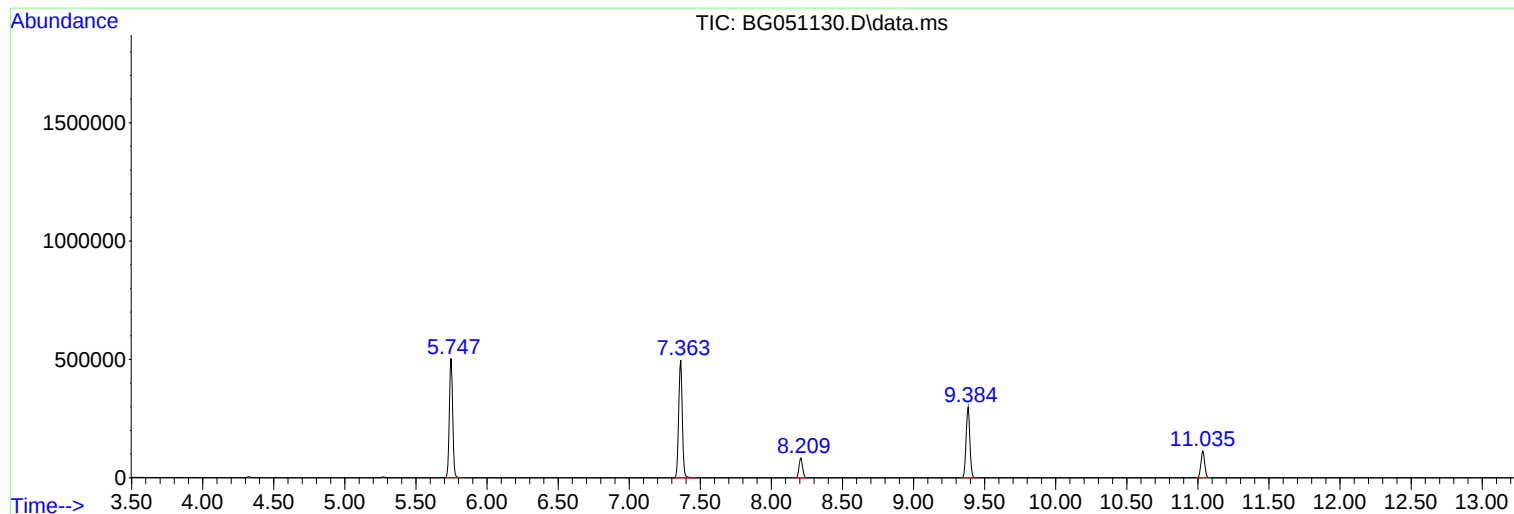

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
Data File : BG051130.D  
Acq On : 19 Nov 2021 19:57  
Operator : CG/JU  
Sample : PB140900BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140900BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
Data File : BG051130.D  
Acq On : 19 Nov 2021 19:57  
Operator : CG/JU  
Sample : PB140900BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140900BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|