


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
 Data File : BG051118.D
 Acq On : 19 Nov 2021 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 16:26:22 2021

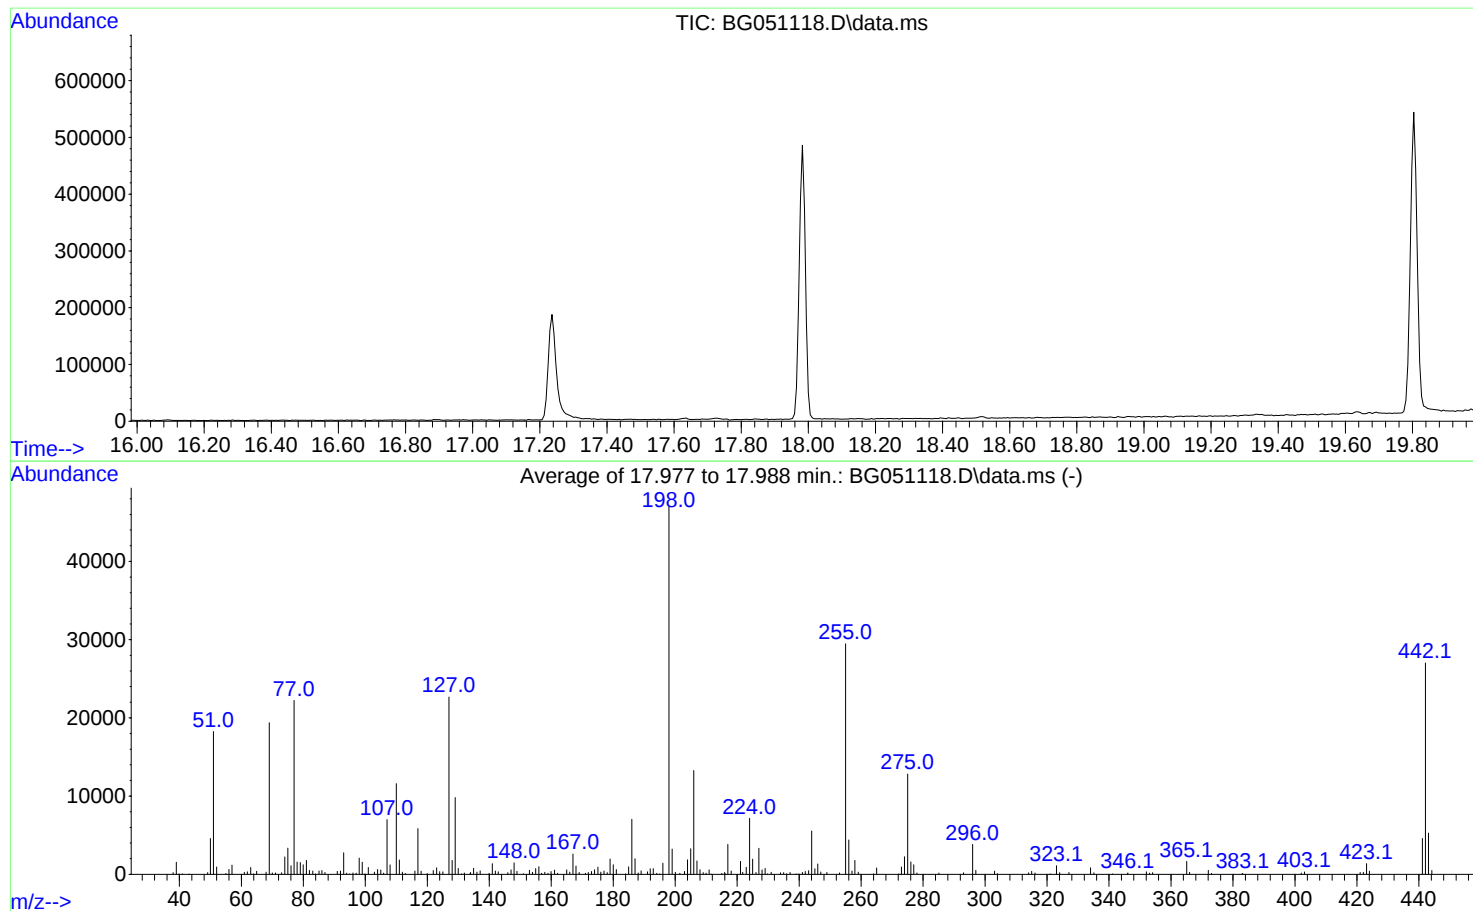




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	18261	PASS
68	69	0.00	2	1.4	280	PASS
69	198	0.00	100	41.2	19380	PASS
70	69	0.00	2	1.0	192	PASS
127	198	10	80	48.2	22664	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47016	PASS
199	198	5	9	6.9	3239	PASS
275	198	10	60	27.3	12824	PASS
365	198	1	100	3.5	1655	PASS
441	198	0.01	100	9.8	4587	PASS
442	442	50	100	100.0	27016	PASS
443	442	15	24	19.5	5275	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051118.D
Acq On : 19 Nov 2021 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:52:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:48:56 2021
Response via : Initial Calibration

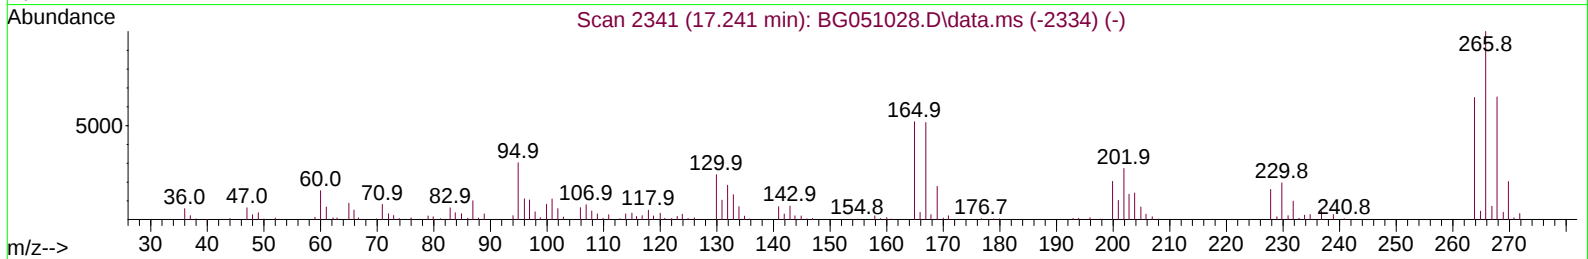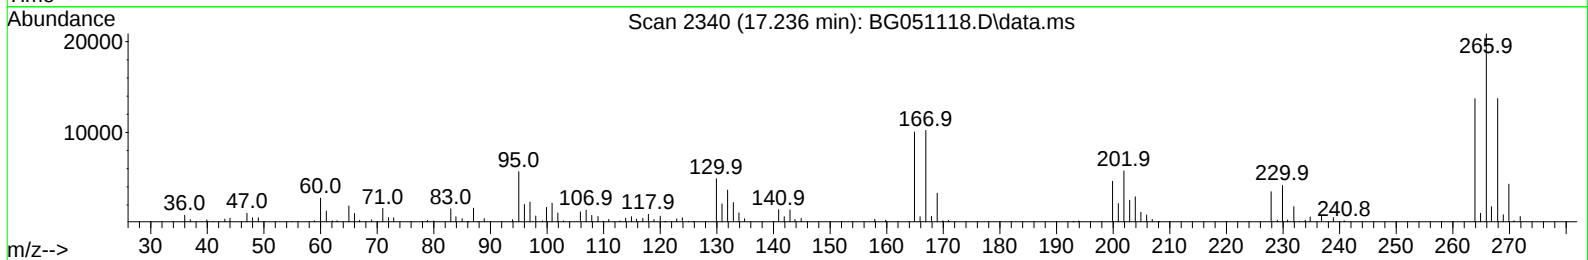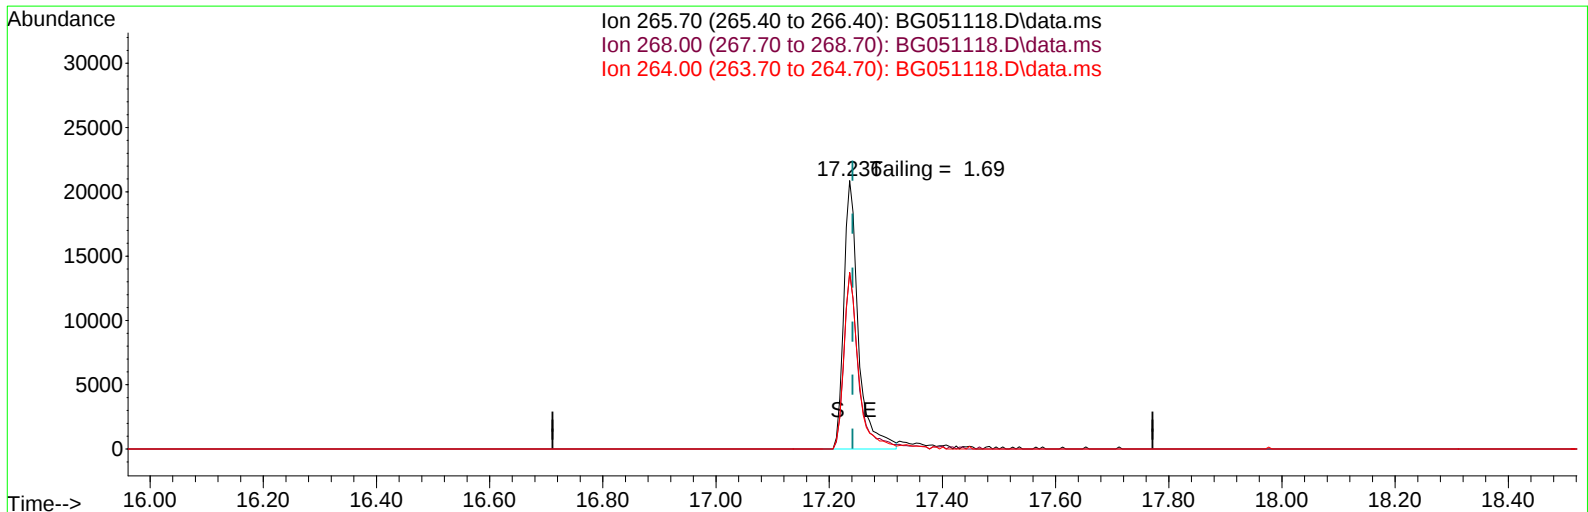

TIC: BG051118.D\data.ms

(70) Pentachlorophenol (C)

17.236min (-0.005) 4732.60 ng




response 37355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.76
264.00	61.30	65.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111921\
Data File : BG051118.D
Acq On : 19 Nov 2021 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:52:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:48:56 2021
Response via : Initial Calibration

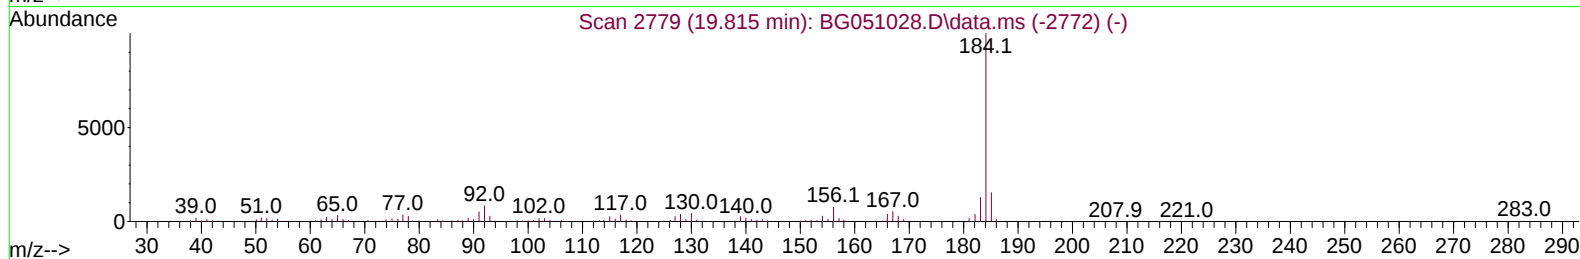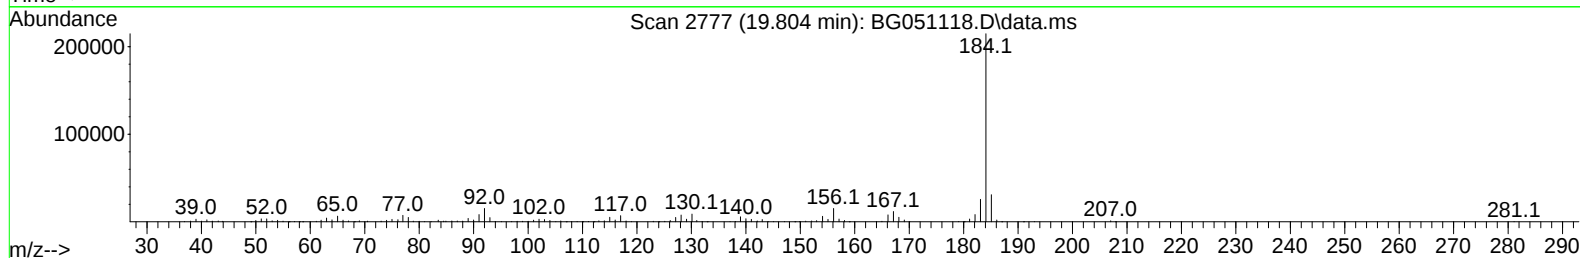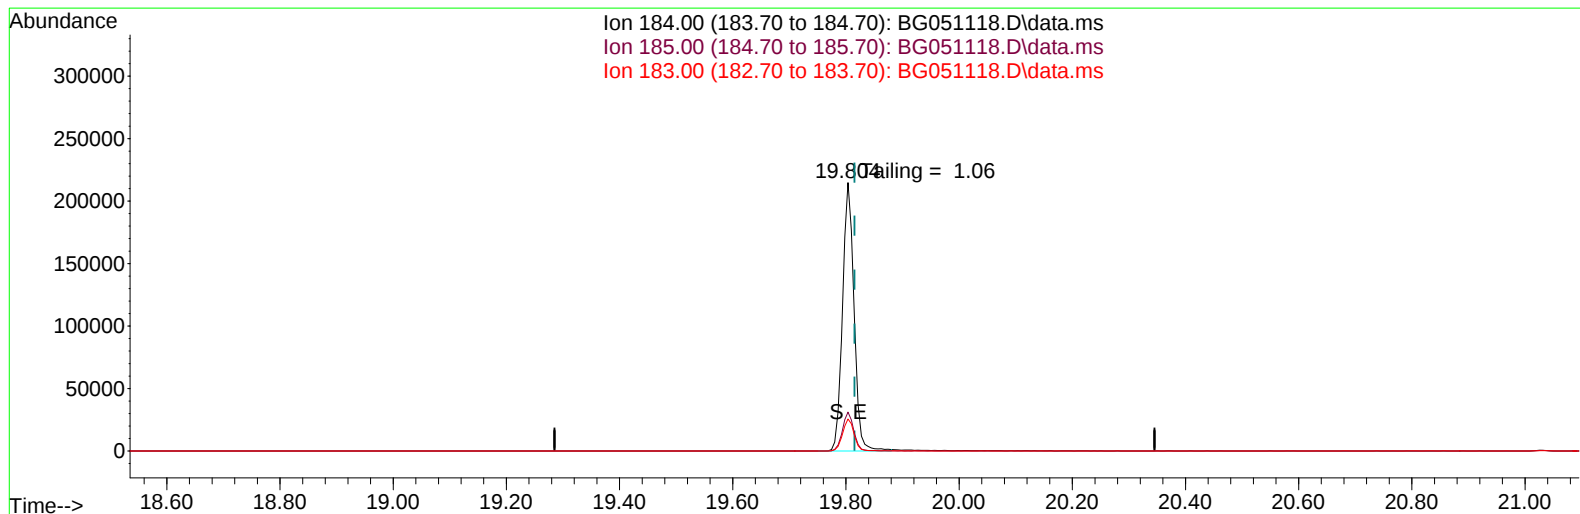

TIC: BG051118.D\data.ms

(77) Benzidine

19.804min (-0.011) 0.00 ng

response 306174

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.48
183.00	11.70	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2021	BNA_G	BG051118.D
Compound Name	Response	Retention Time
DDT	160929	21.03
DDD	2163	20.58
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2163	163092	1.33

Instrument :
BNA_G
ClientSampleId :
DFTPP