
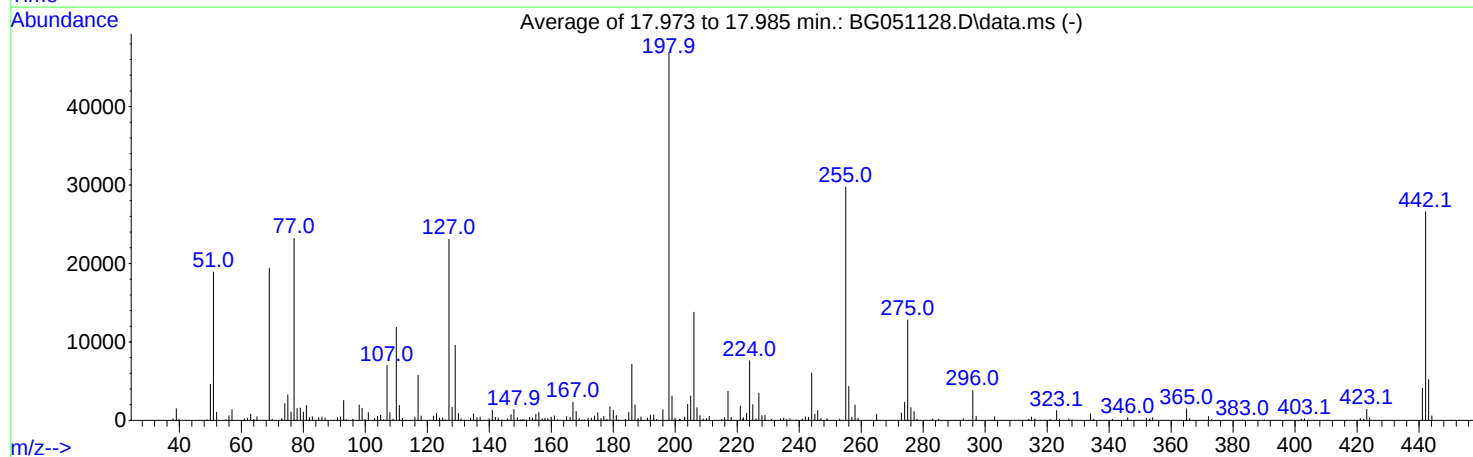


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
 Data File : BG051128.D  
 Acq On : 19 Nov 2021 18:35  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Nov 19 16:26:22 2021

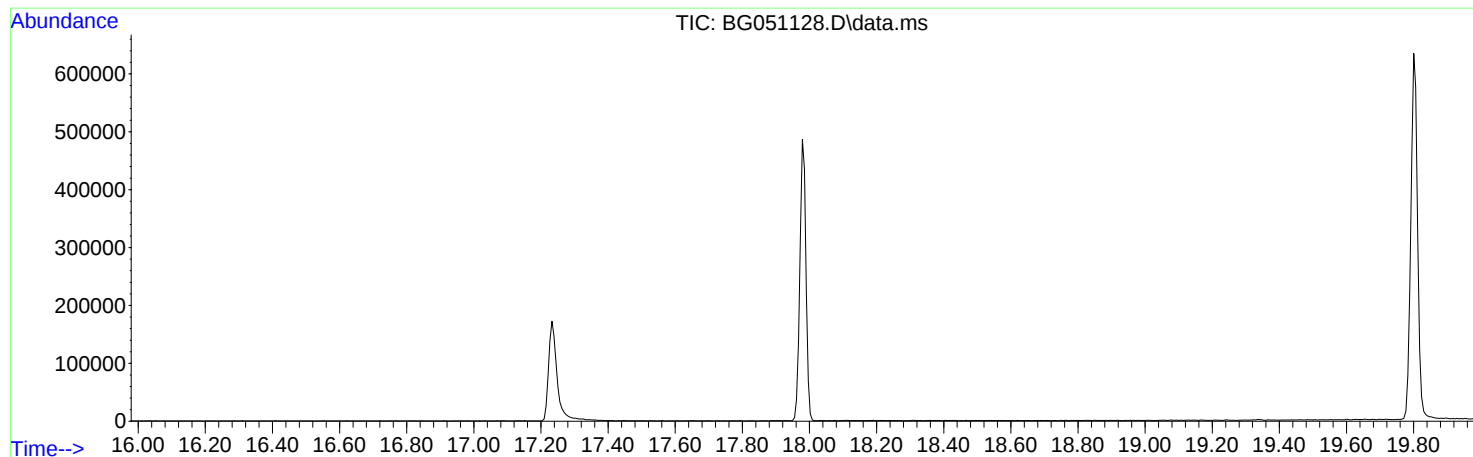




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.3         | 18909      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 41.4         | 19395      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 134        | PASS                |
| 127            | 198             | 10              | 80              | 49.2         | 23096      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 46896      | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 3109       | PASS                |
| 275            | 198             | 10              | 60              | 27.3         | 12804      | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 1466       | PASS                |
| 441            | 198             | 0.01            | 100             | 8.8          | 4122       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 26591      | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 5179       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
Data File : BG051128.D  
Acq On : 19 Nov 2021 18:35  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Nov 19 19:10:38 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 19 16:26:22 2021  
Response via : Initial Calibration

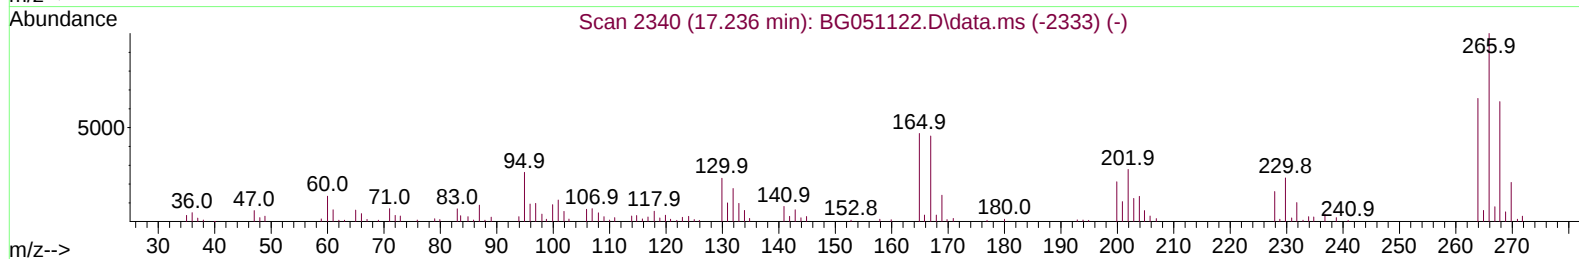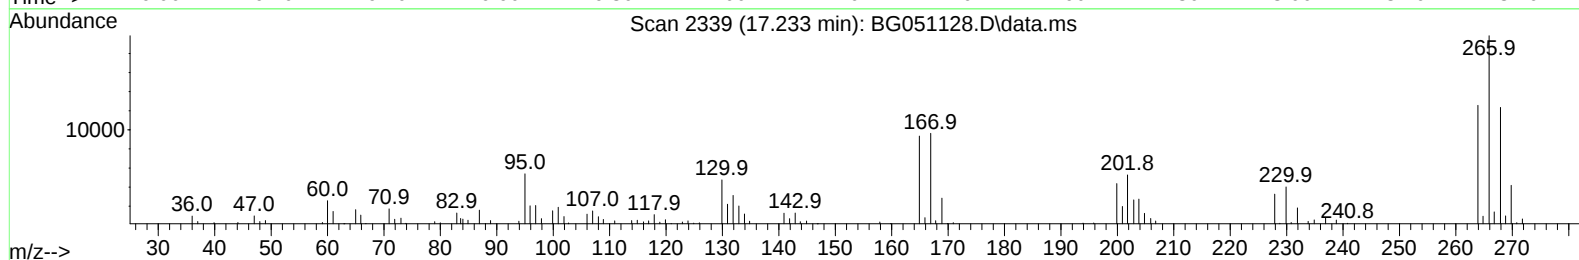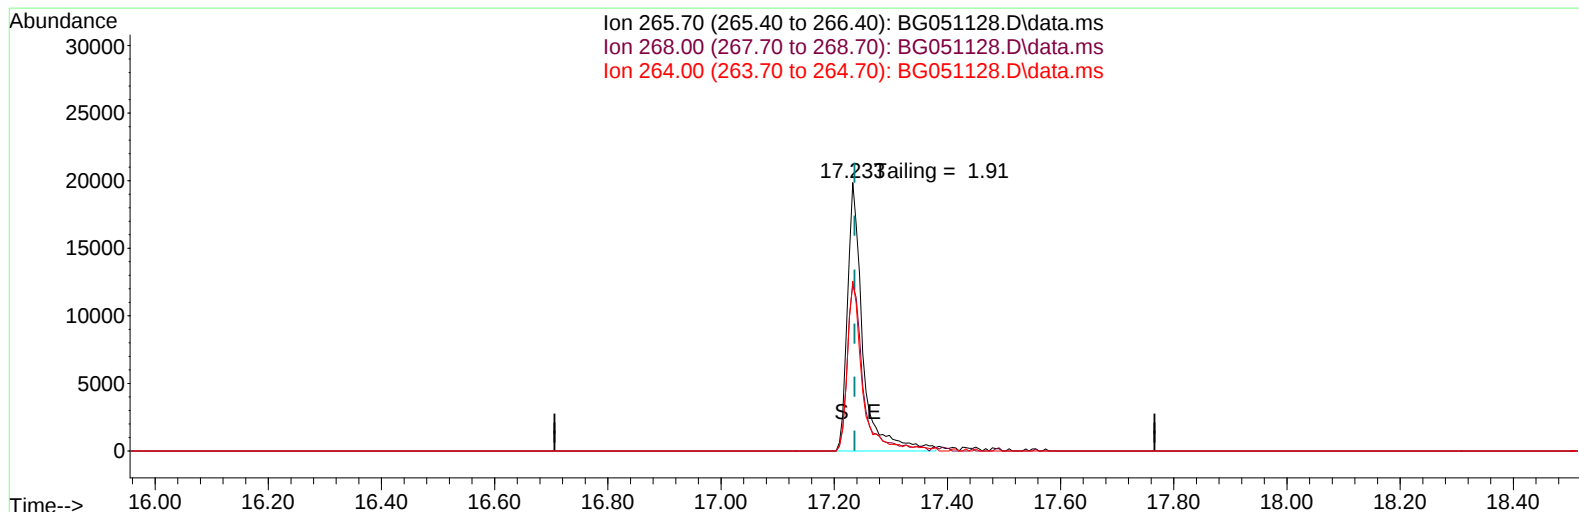

TIC: BG051128.D\data.ms

**(70) Pentachlorophenol (C)**

17.233min (-0.003) 27828.96 ng




response 36995

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 62.18  |
| 264.00 | 61.30  | 63.27  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111921\  
Data File : BG051128.D  
Acq On : 19 Nov 2021 18:35  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Nov 19 19:10:38 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 19 16:26:22 2021  
Response via : Initial Calibration

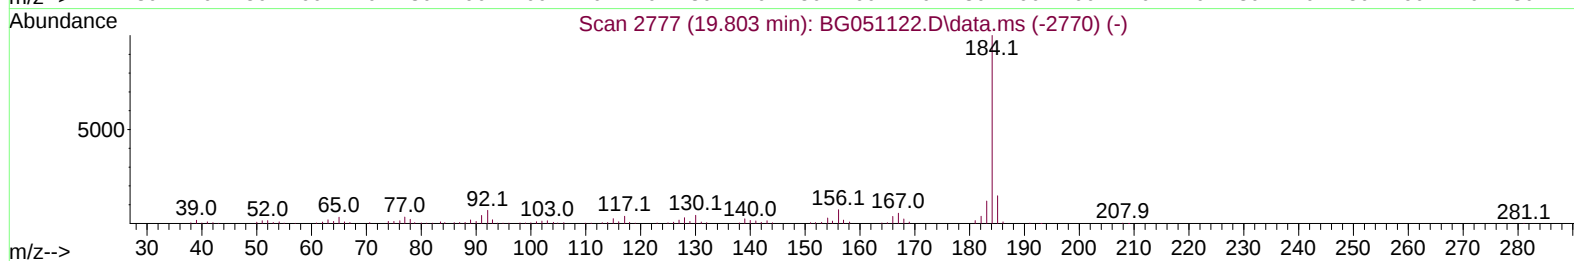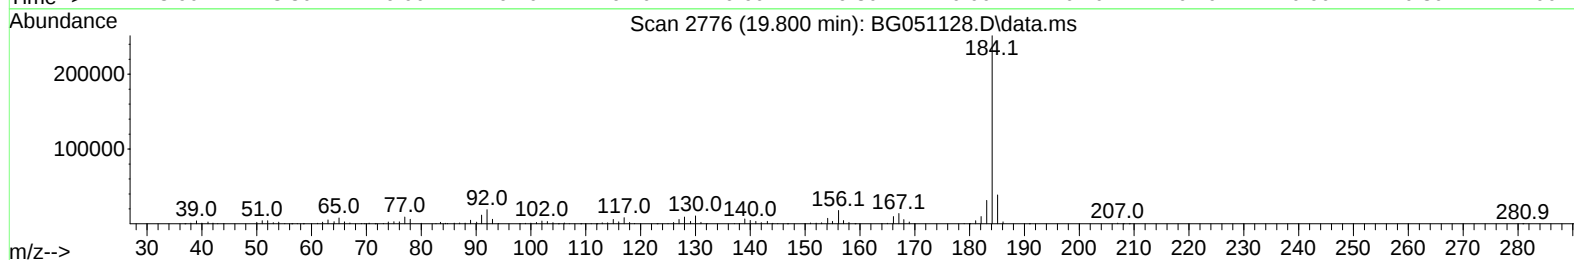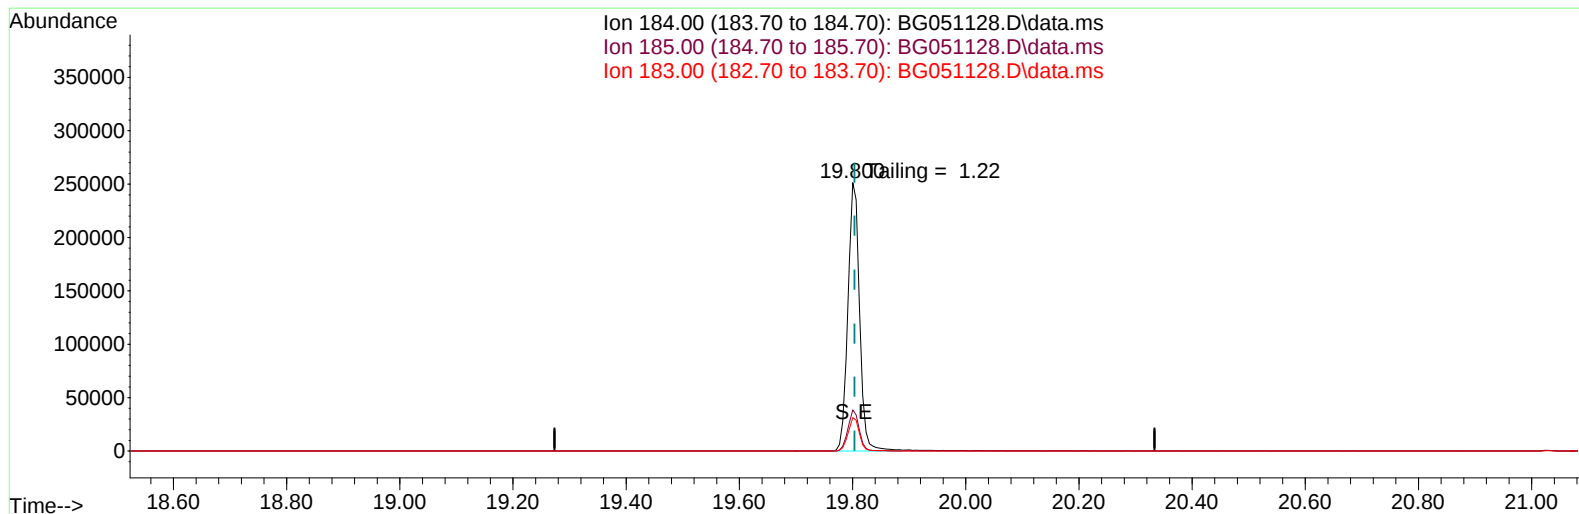

TIC: BG051128.D\data.ms

**(77) Benzidine**

**19.800min (-0.003) 0.00 ng**

**response 358393**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 15.36  |
| 183.00 | 11.70  | 12.48  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/19/2021    | BNA_G            | BG051128.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 164494           | 21.028             |
| DDD           | 5732             | 20.582             |
| DDE           | 0                | 19.9               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5732          | 170226           | 3.37               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP