


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111925\
Data File : BG064810.D
Acq On : 19 Nov 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

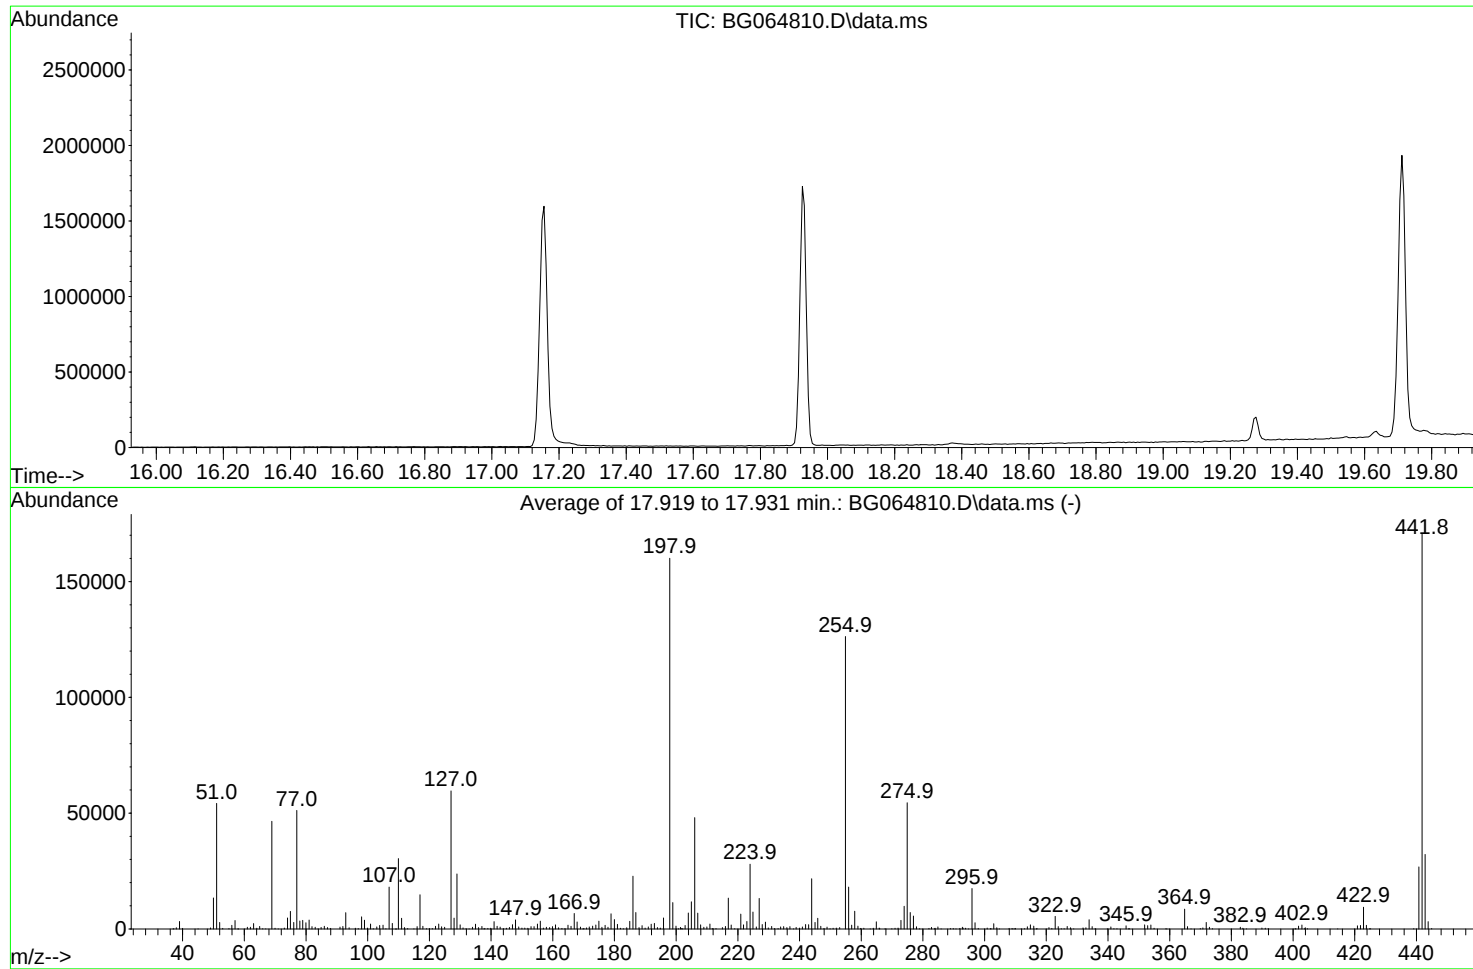




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	46445	PASS
70	69	0.00	2	0.7	305	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160045	PASS
199	198	5	9	7.1	11337	PASS
365	198	1	100	5.4	8571	PASS
441	443	0.01	150	83.2	26770	PASS
442	442	100	100	100.0	170515	PASS
443	442	15	24	18.9	32160	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111925\
Data File : BG064810.D
Acq On : 19 Nov 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:27:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

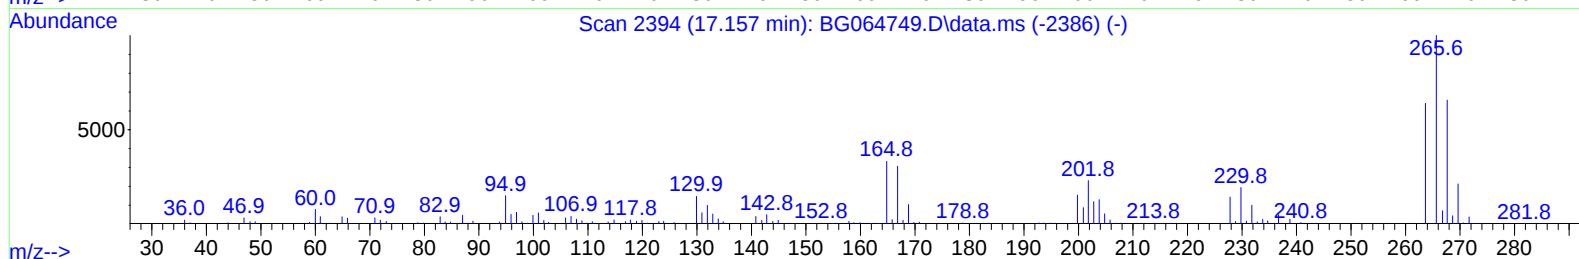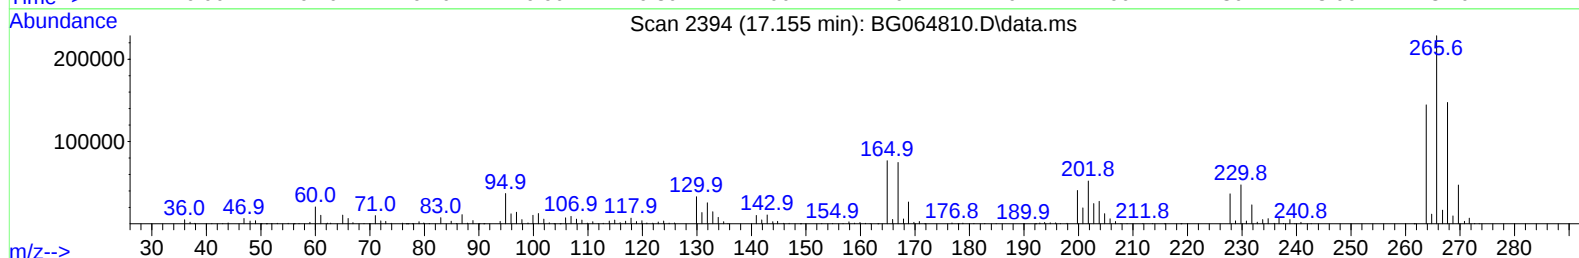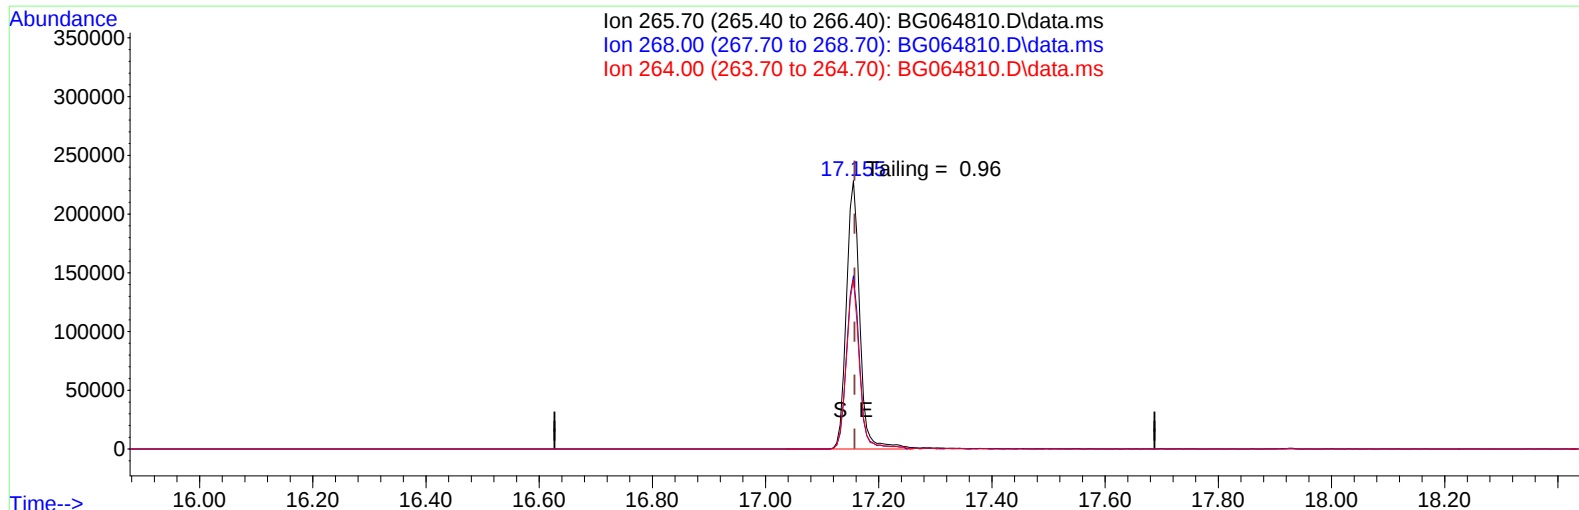

TIC: BG064810.D\data.ms

(70) Pentachlorophenol (C)

17.155min (-0.002) 646429.46 ng




response 375770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	68.72
264.00	64.00	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111925\
Data File : BG064810.D
Acq On : 19 Nov 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:27:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

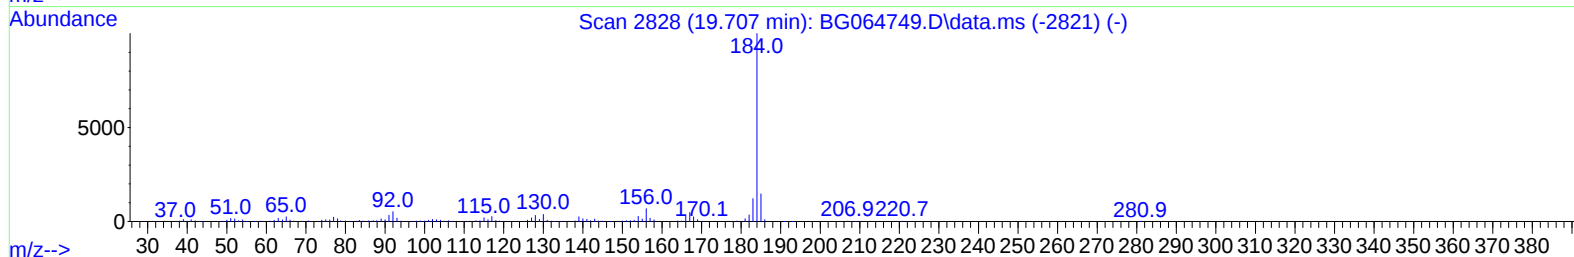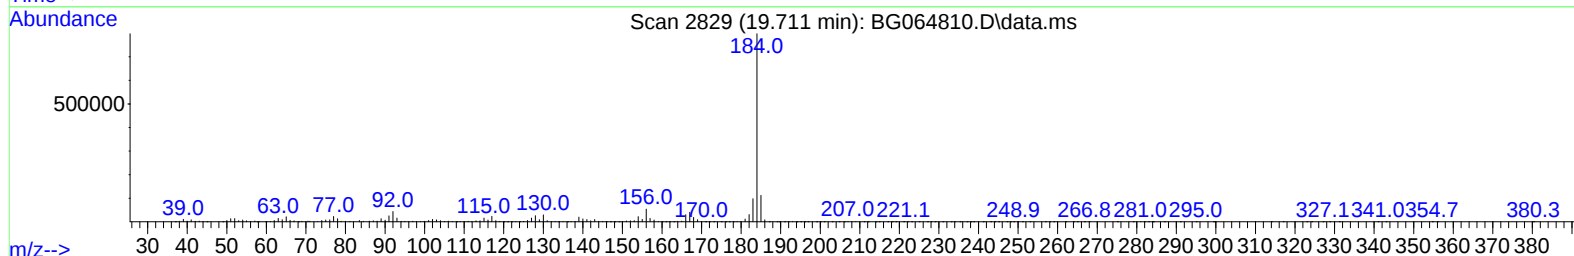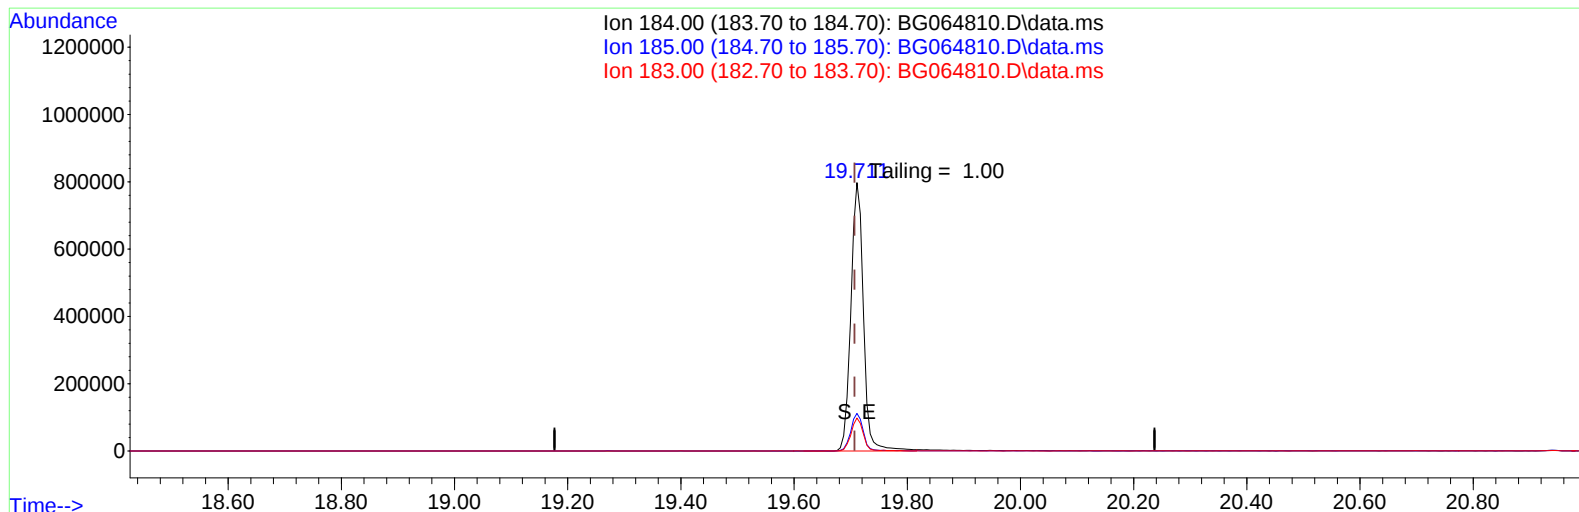

TIC: BG064810.D\data.ms

(77) Benzidine

19.711min (+ 0.004) 77987.81 ng

response 1242545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.03
183.00	12.20	12.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2025	BNA_G	<u>BG064810.D</u>
Compound Name	Response	Retention Time
DDT	751884	20.939
DDD	23058	20.498
DDE	2406	19.999
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25464	777348	3.28

Instrument :
BNA_G
ClientSampleId :
DFTPP