
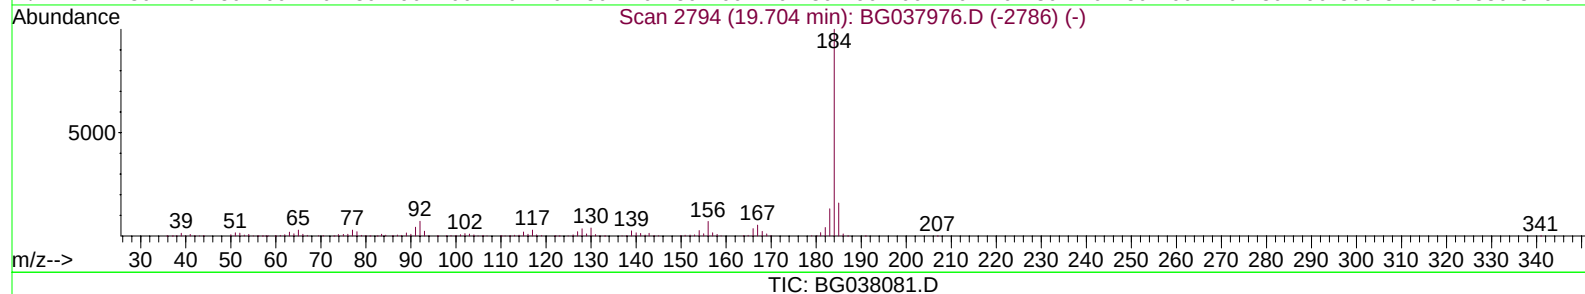
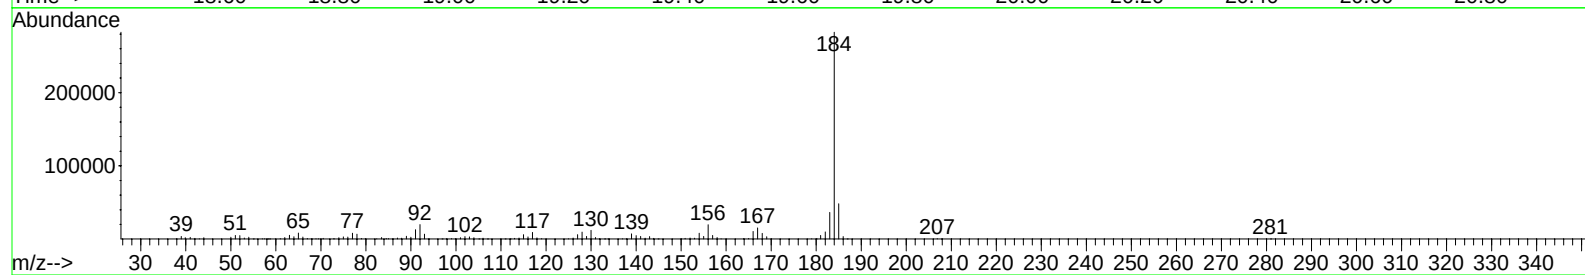


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112018\
Data File : BG038081.D
Acq On : 20 Nov 2018 12:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 17:02:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

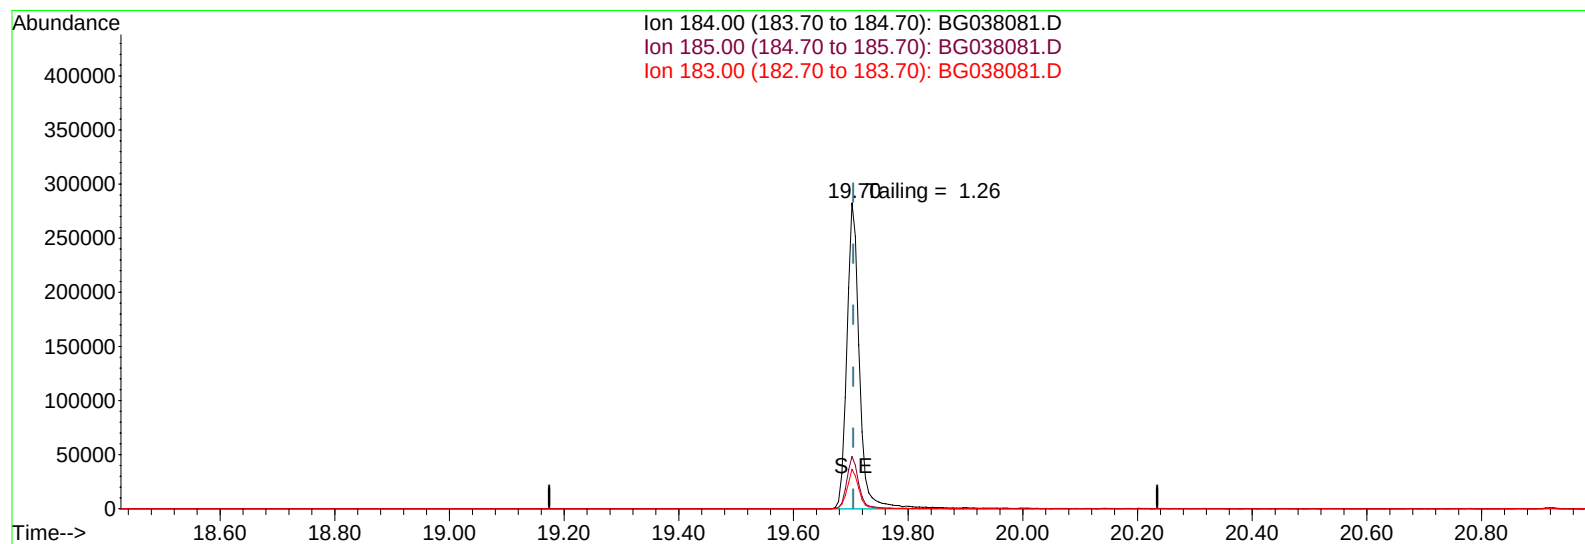

TIC: BG038081.D

(77) Benzidine




19.702min (-0.002) 0.00ng

response 428780

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.05
183.00	12.70	12.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112018\
Data File : BG038081.D
Acq On : 20 Nov 2018 12:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 17:02:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

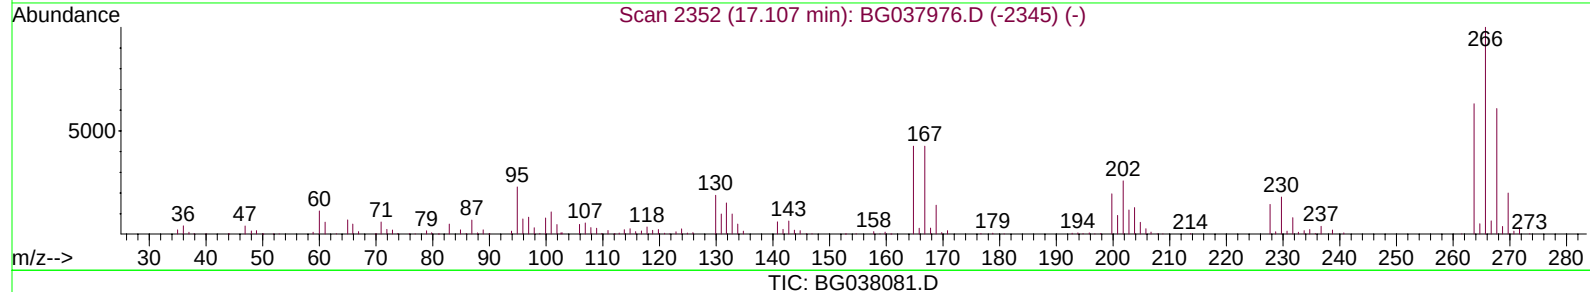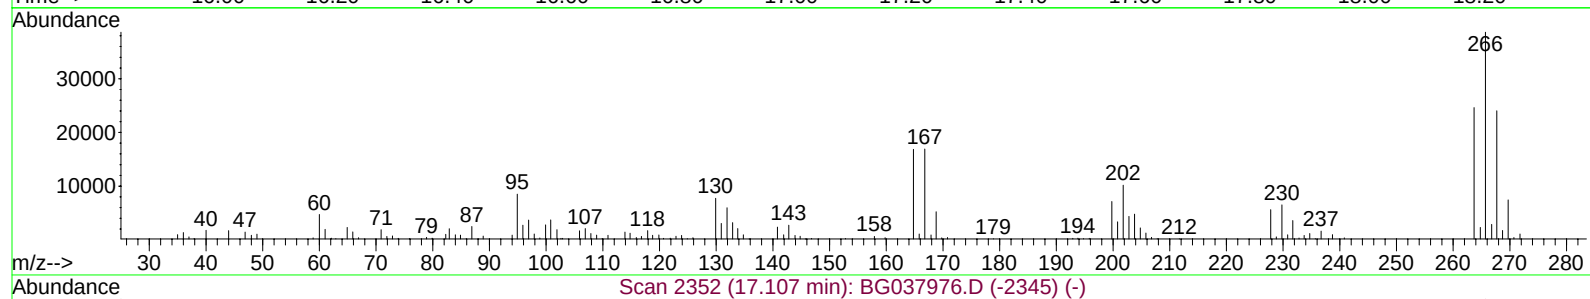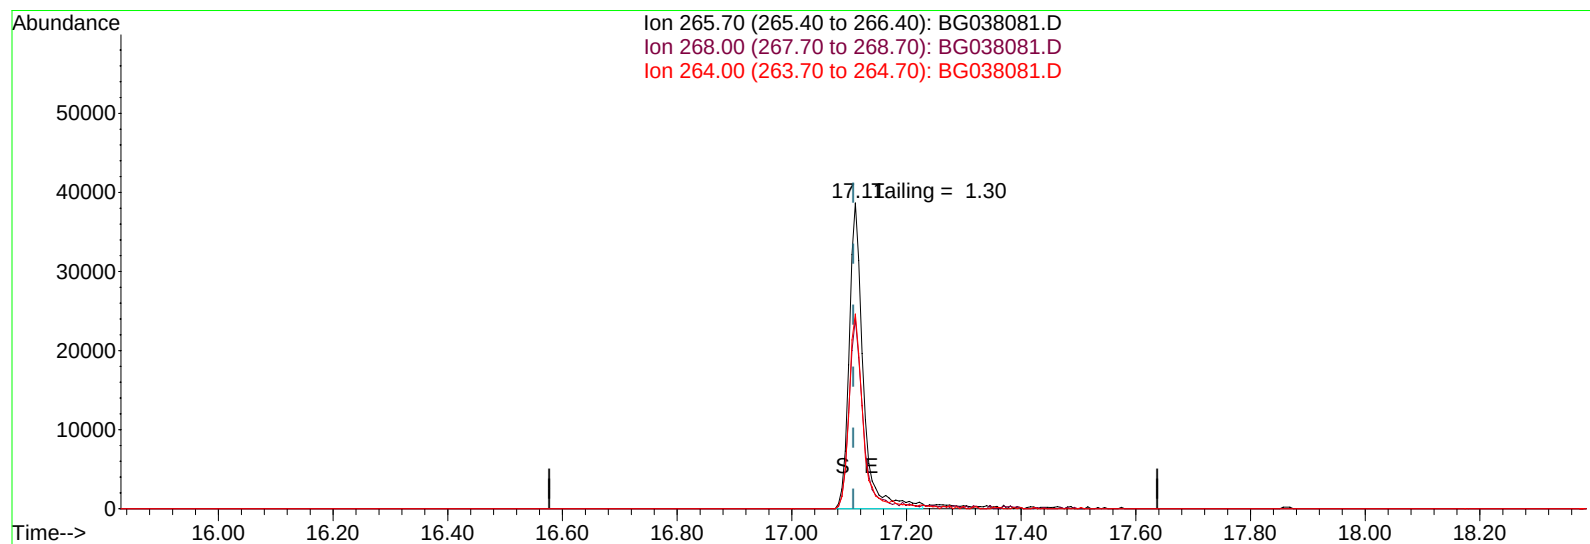

(70) Pentachlorophenol (C)

17.111min (+0.004) 25044.97ng

response 66484

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.63
264.00	73.60	63.71
0.00	0.00	0.00