

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112018\
 Data File : BG038108.D
 Acq On : 21 Nov 2018 7:14
 Operator : JU/SJ
 Sample : J6006-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RS-CON-WALL-2

Quant Time: Nov 21 10:52:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	38373	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	168199	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	107565	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	245189	20.00	ng	0.00
76) Chrysene-d12	21.75	240	234757	20.00	ng	0.00
87) Perylene-d12	25.07	264	223256	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	252113	113.44	ng	0.00
7) Phenol-d6	7.23	99	311743	98.26	ng	0.00
23) Nitrobenzene-d5	9.26	82	268683	85.51	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	133998	109.23	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	588859	79.75	ng	0.00
79) Terphenyl-d14	20.07	244	916654	91.88	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112018\
Data File : BG038108.D
Acq On : 21 Nov 2018 7:14
Operator : JU/SJ
Sample : J6006-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RS-CON-WALL-2

Quant Time: Nov 21 10:52:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

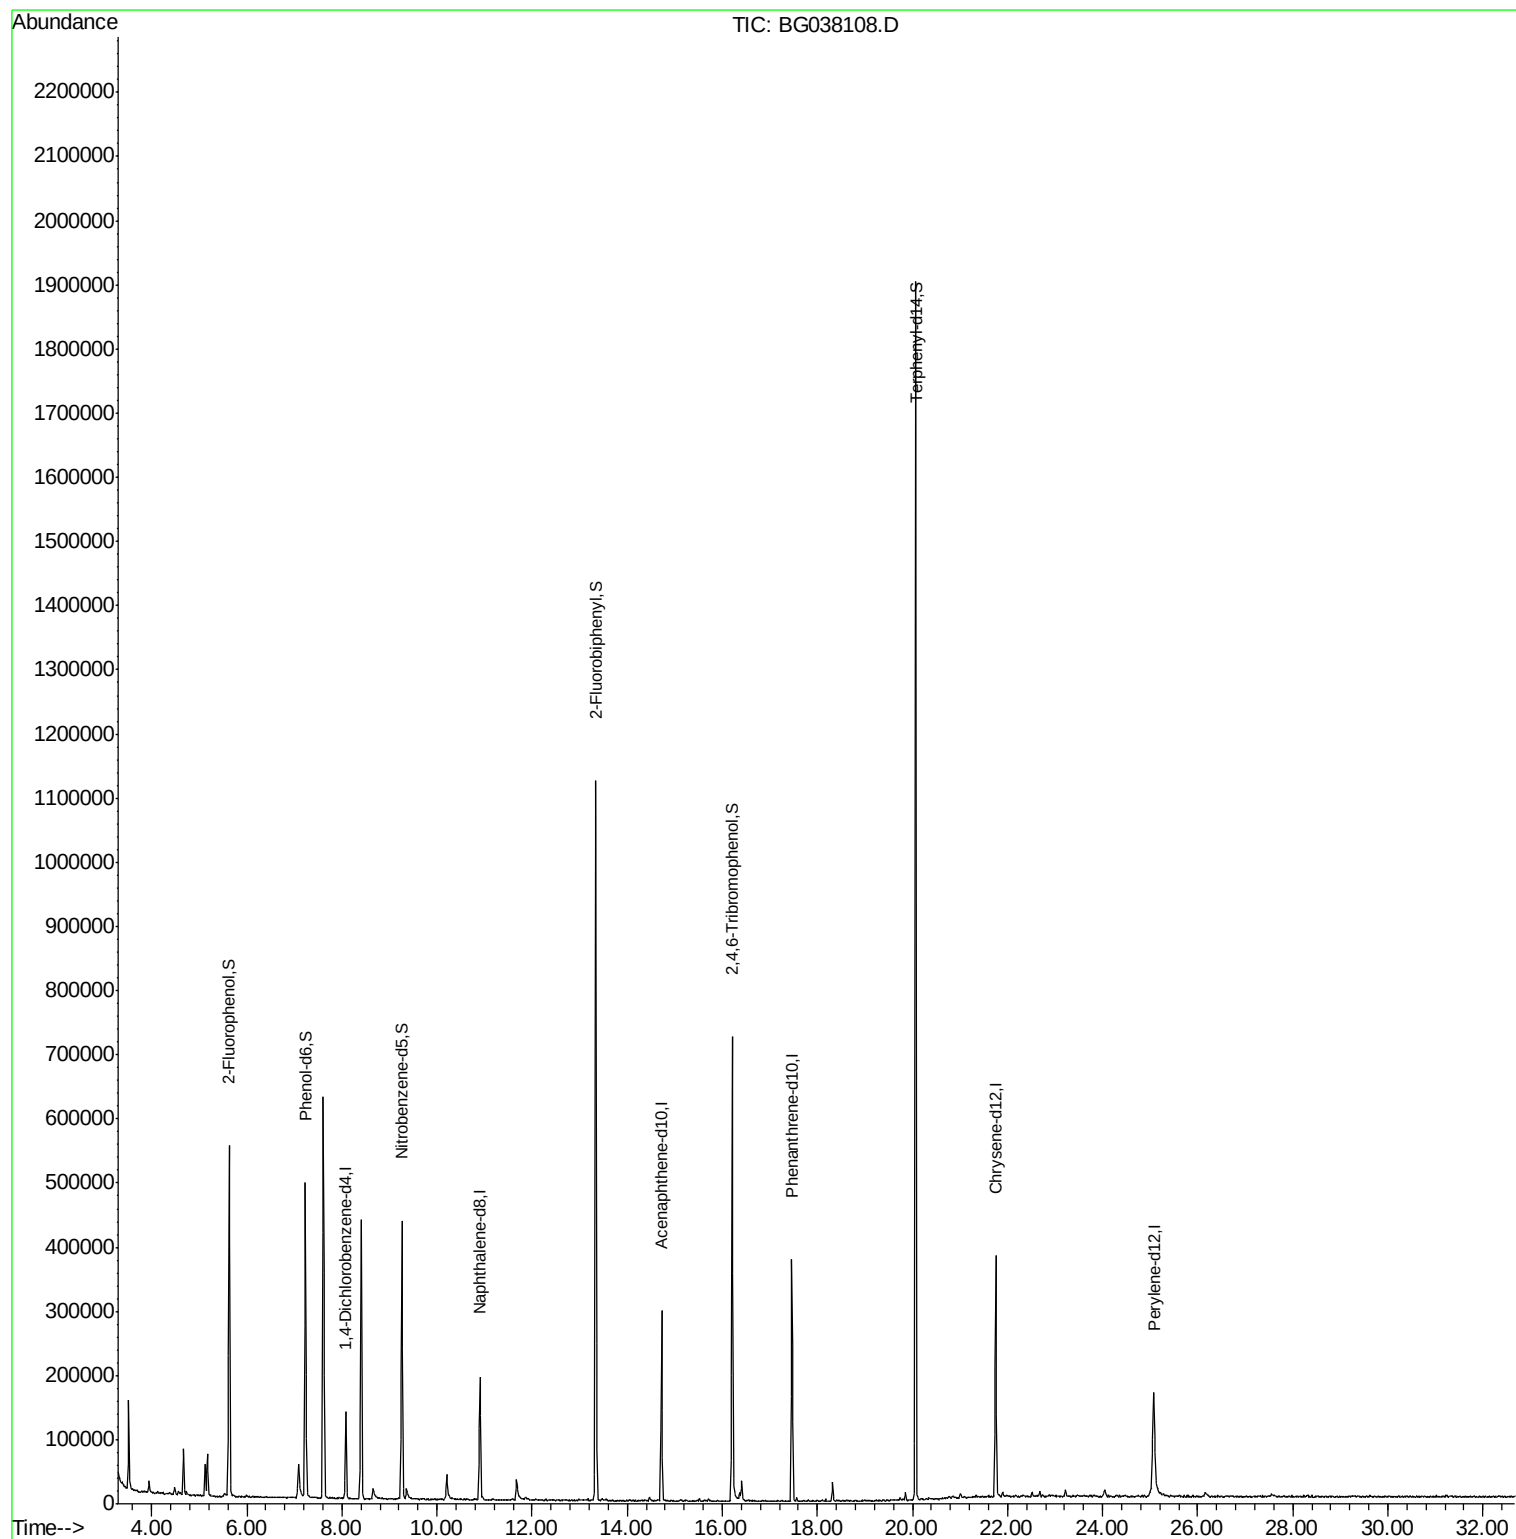

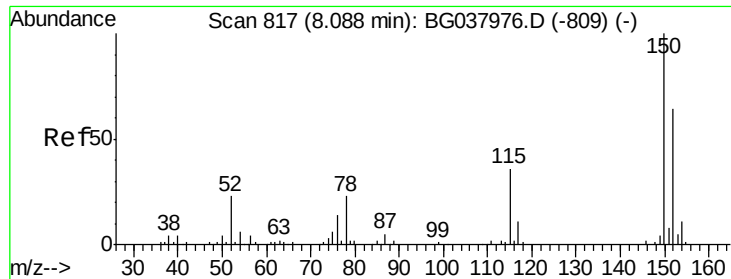


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.08 min Scan# 816
 Delta R.T. -0.01 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Instrument :
 BNA_G
 ClientSampleId :
 RS-CON-WALL-2

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.5	126.0	189.0
115	56.2	45.5	68.3



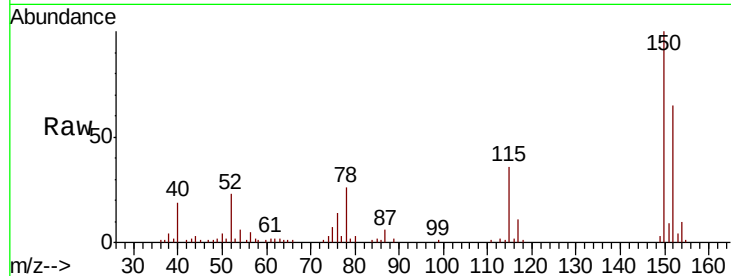


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

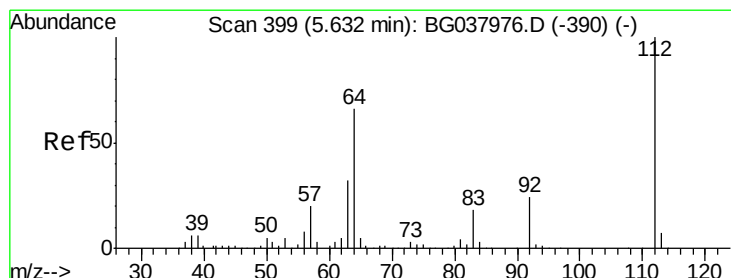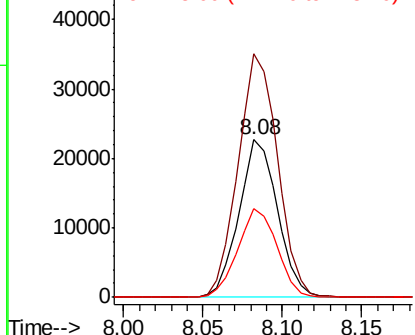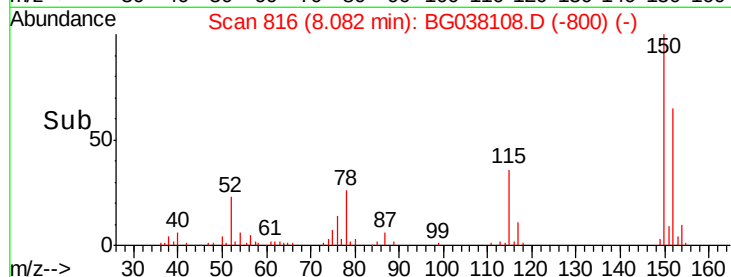

#5

2-Fluorophenol
 Concen: 113.436 ng
 RT: 5.63 min Scan# 399
 Delta R.T. 0.00 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.8	53.1	79.7
63	34.8	27.3	40.9


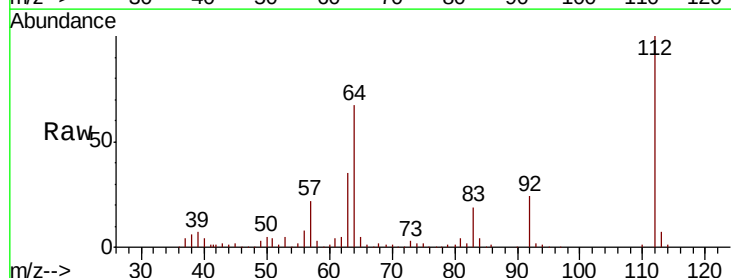



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

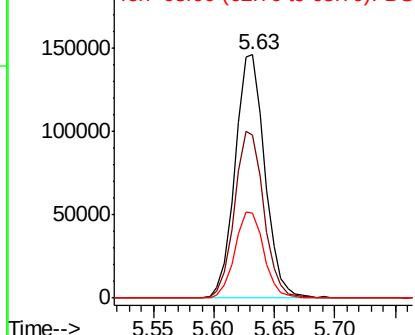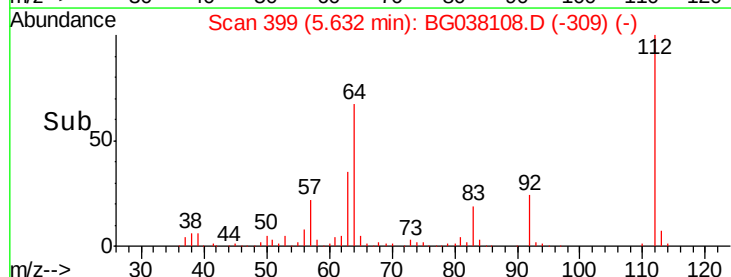

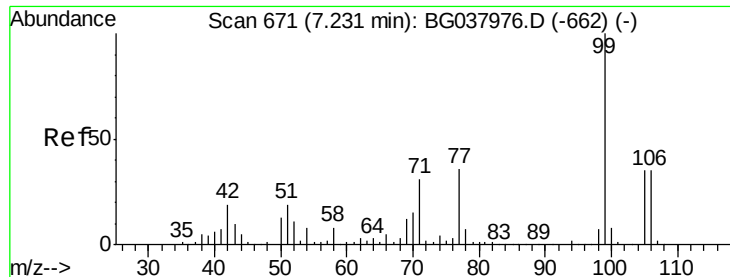

#7

Phenol-d6

Concen: 98.264 ng

RT: 7.23 min Scan# 671

Delta R.T. -0.00 min

Lab File: BG038108.D

Acq: 21 Nov 2018 7:14

Instrument :

BNA_G

ClientSampleId :

RS-CON-WALL-2


Tot Ion: 99 Resp: 311743

Ion Ratio Lower Upper




99 100

42 19.8 15.0 22.4

71 32.2 25.5 38.3

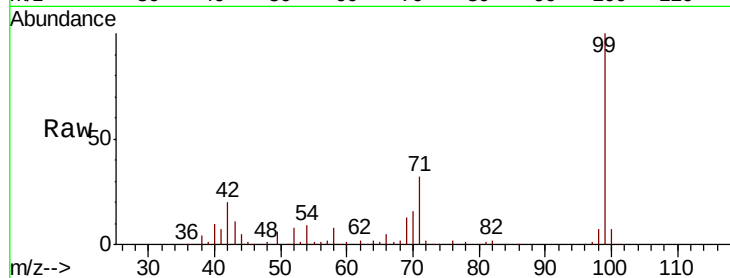

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

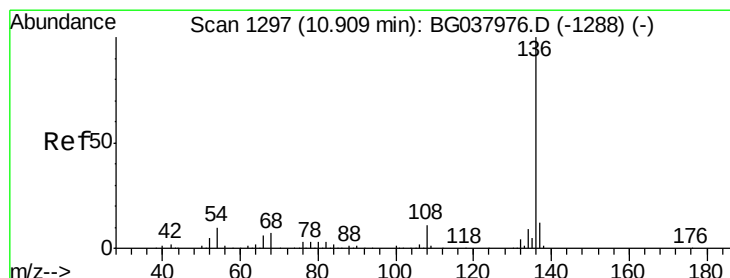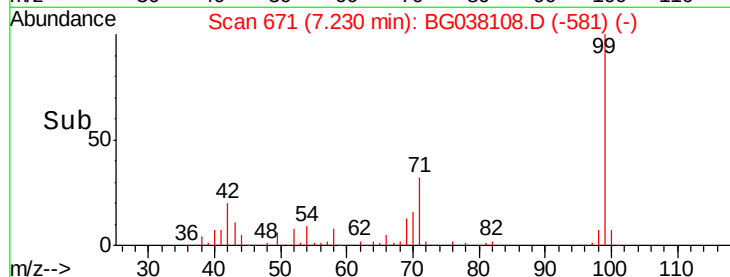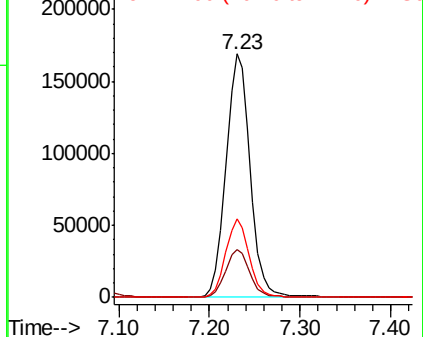

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BG038108.D

Acq: 21 Nov 2018 7:14

Tgt Ion: 136 Resp: 168199


Ion Ratio Lower Upper

136 100



137 11.3 9.6 14.4


54 11.2 7.9 11.9

68 6.8 4.8 7.2

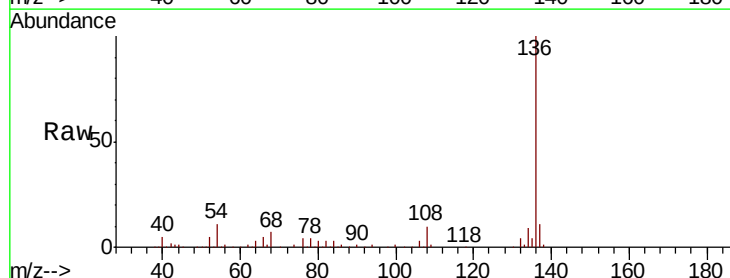

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

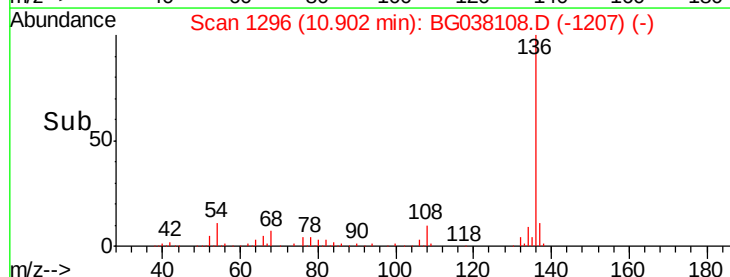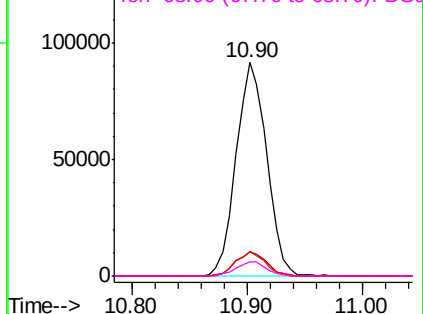


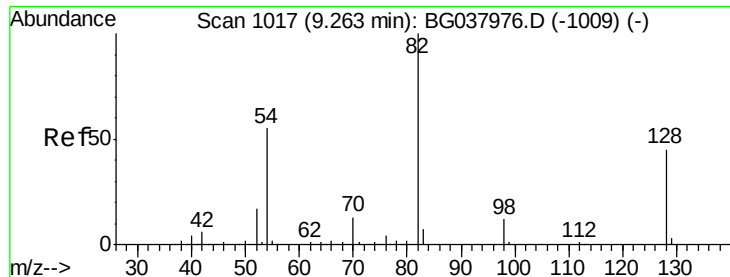




#23
 Nitrobenzene-d5
 Concen: 85.510 ng
 RT: 9.26 min Scan# 1017
 Delta R.T. -0.00 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Instrument :
 BNA_G
 ClientSampleId :
 RS-CON-WALL-2

Tot Ion	82	Resp	268683
Ion Ratio	100	Lower	Upper
128	42.5	34.6	51.8
54	55.2	45.3	67.9

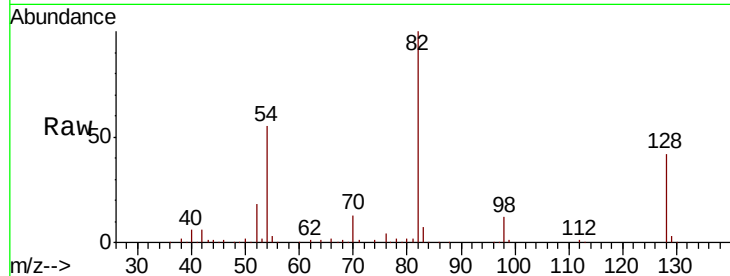


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

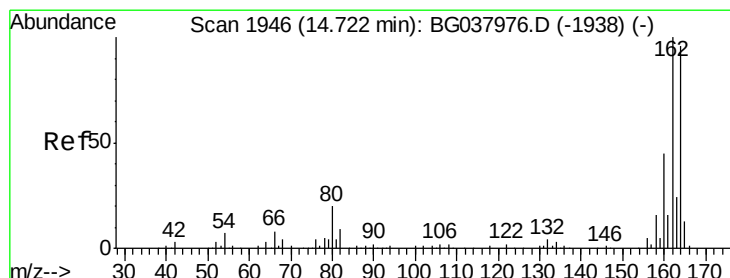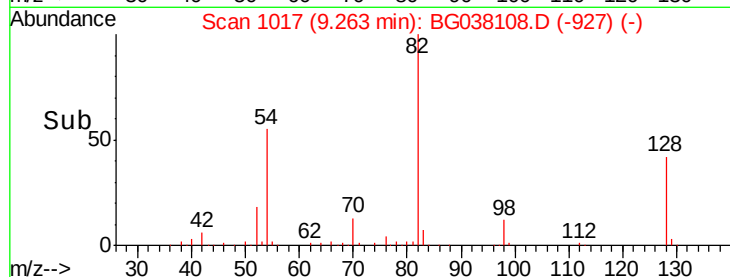
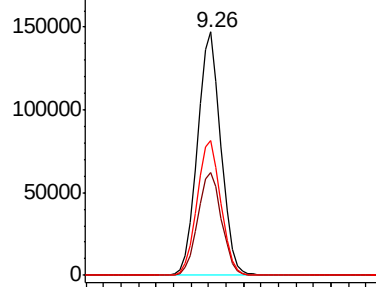



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.72 min Scan# 1946
 Delta R.T. -0.00 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Tgt Ion	164	Resp	107565
Ion Ratio	100	Lower	Upper
162	108.0	81.3	121.9
160	45.8	36.3	54.5

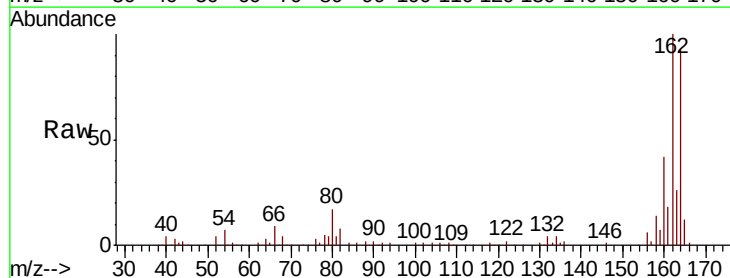

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

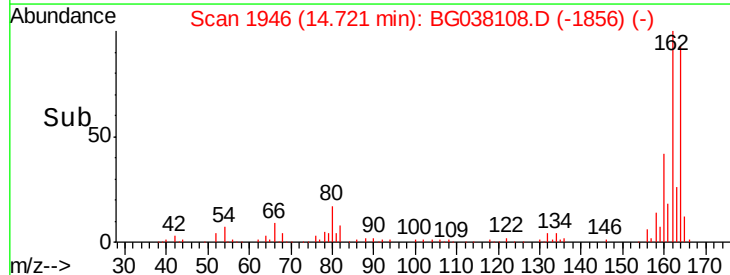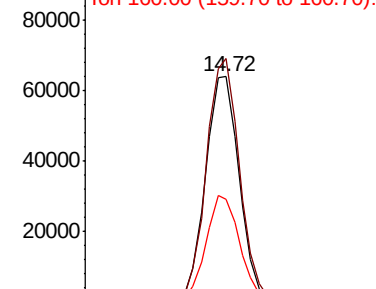


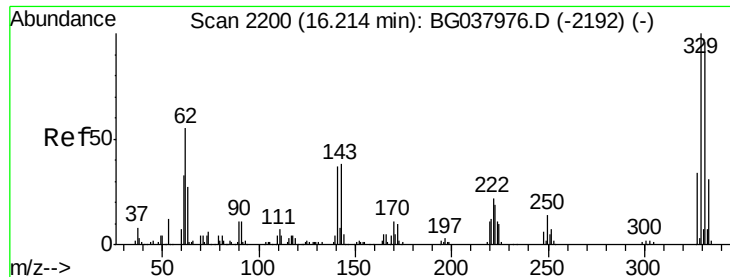

#42
 2,4,6-Tribromophenol
 Concen: 109.230 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. -0.01 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Instrument :
 BNA_G
 ClientSampleId :
 RS-CON-WALL-2

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	78.4	117.6
141	42.9	32.2	48.2



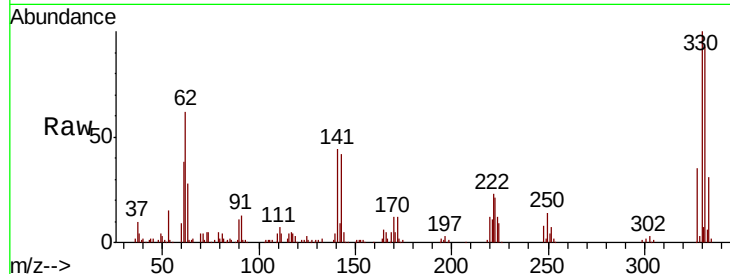


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

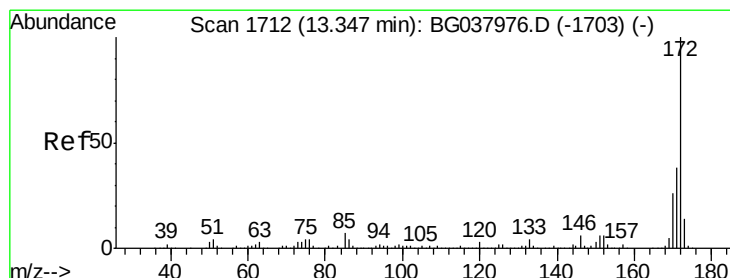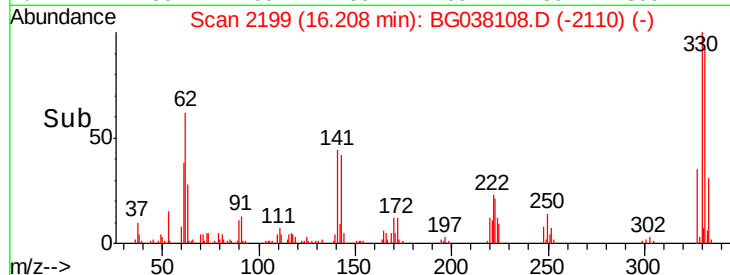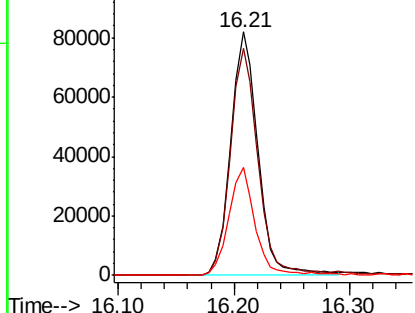

#45
 2-Fluorobiphenyl
 Concen: 79.755 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BG038108.D
 Acq: 21 Nov 2018 7:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	31.0	46.4
170	24.2	20.2	30.2


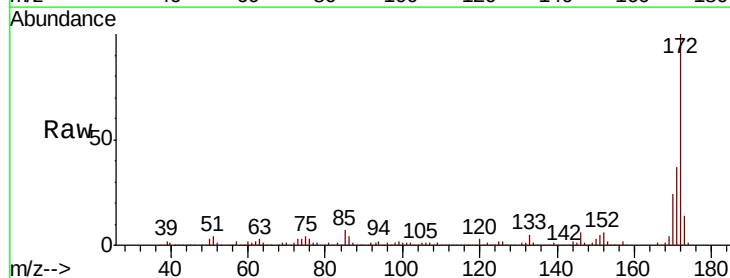



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

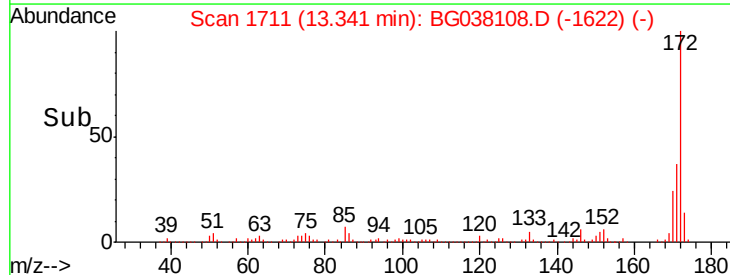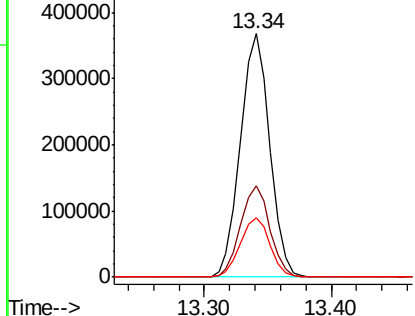


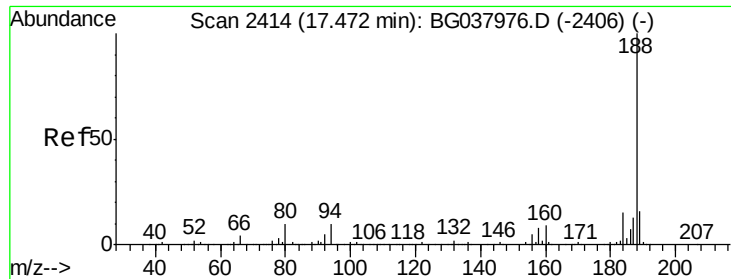




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BG038108.D
Acq: 21 Nov 2018 7:14

Instrument :
BNA_G
ClientSampleId :
RS-CON-WALL-2

Tot Ion:188 Resp: 245189
Ion Ratio Lower Upper
188 100
94 9.4 7.2 10.8
80 10.3 7.7 11.5

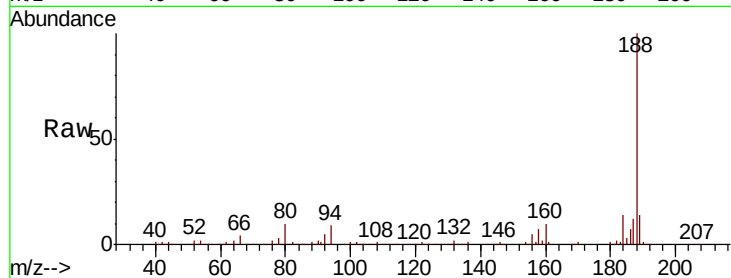


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

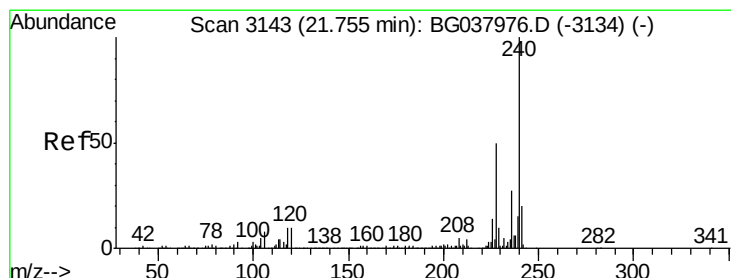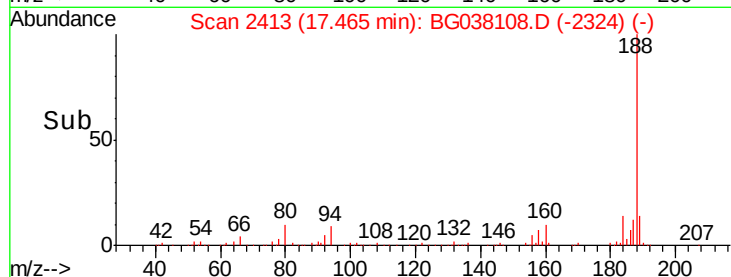
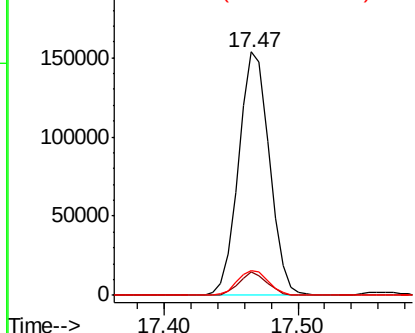



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.75 min Scan# 3142
Delta R.T. -0.01 min
Lab File: BG038108.D
Acq: 21 Nov 2018 7:14

Tgt Ion:240 Resp: 234757
Ion Ratio Lower Upper
240 100
120 10.5 8.1 12.1
236 26.5 21.4 32.0

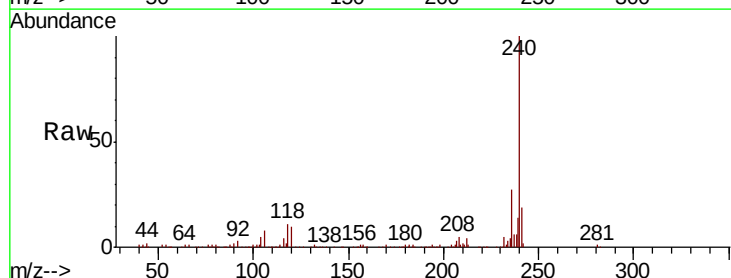

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

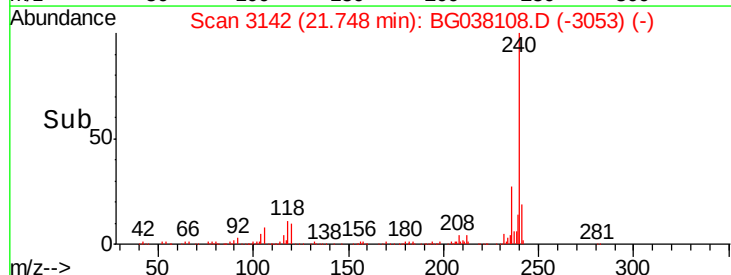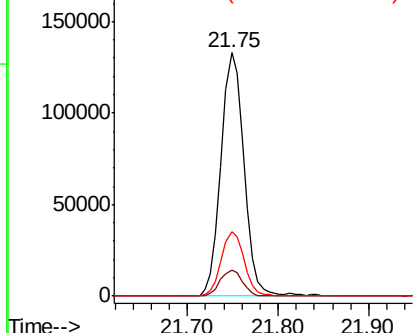

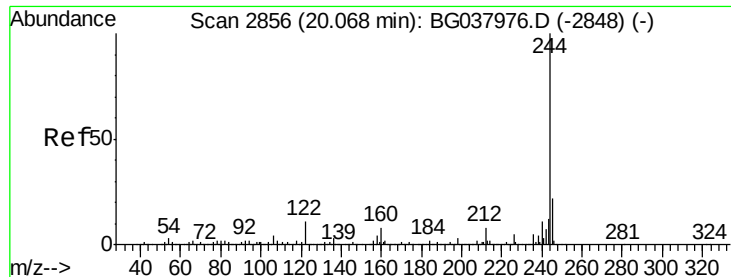

#79

Terphenyl-d14

Concen: 91.878 ng

RT: 20.07 min Scan# 2856

Delta R.T. 0.00 min

Lab File: BG038108.D

Acq: 21 Nov 2018 7:14

Instrument :

BNA_G

ClientSampleId :

RS-CON-WALL-2


Tot Ion:244 Resp: 916654

Ion Ratio Lower Upper

244 100

212 8.1 6.5 9.7




122 10.5 9.0 13.4

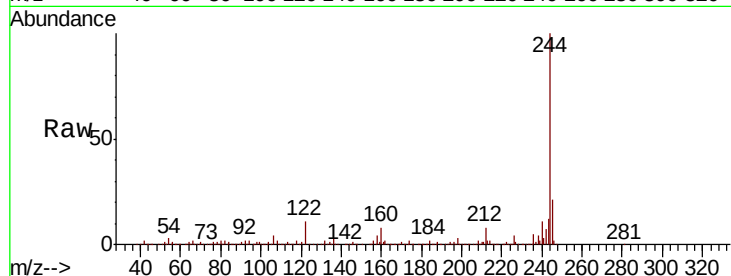

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

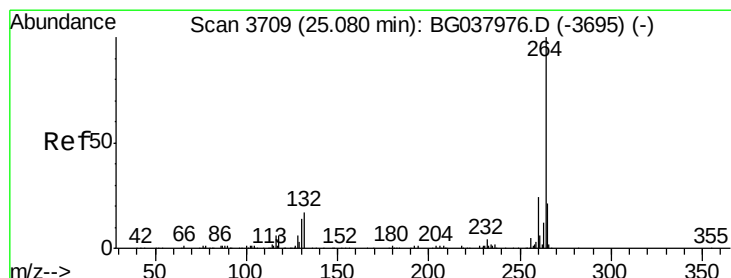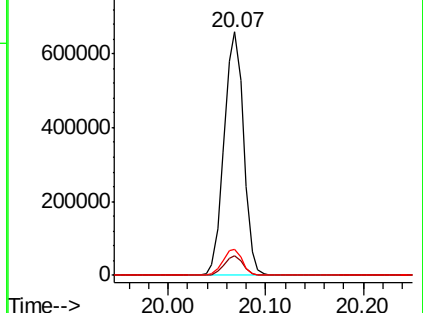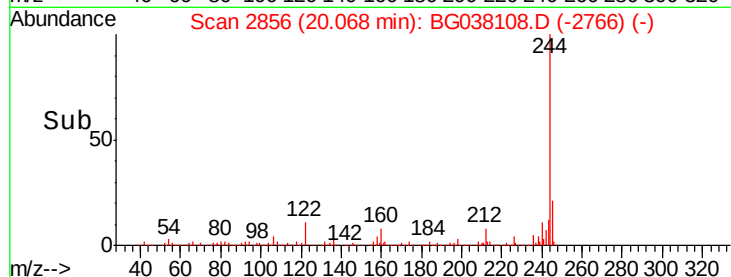

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.07 min Scan# 3708

Delta R.T. -0.01 min

Lab File: BG038108.D

Acq: 21 Nov 2018 7:14


Tgt Ion:264 Resp: 223256

Ion Ratio Lower Upper

264 100

260 22.5 18.2 27.4

265 20.1 17.9 26.9

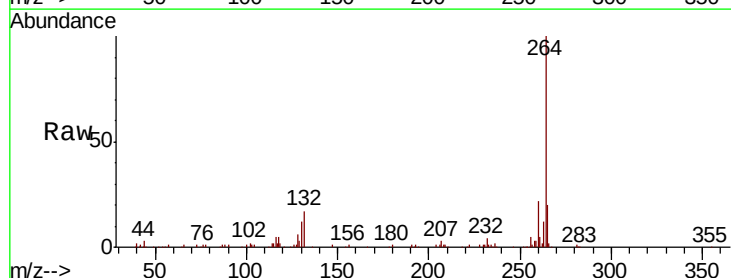

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

