


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112018\  
 Data File : BG038081.D  
 Acq On : 20 Nov 2018 12:12  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG111318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Nov 13 16:39:28 2018

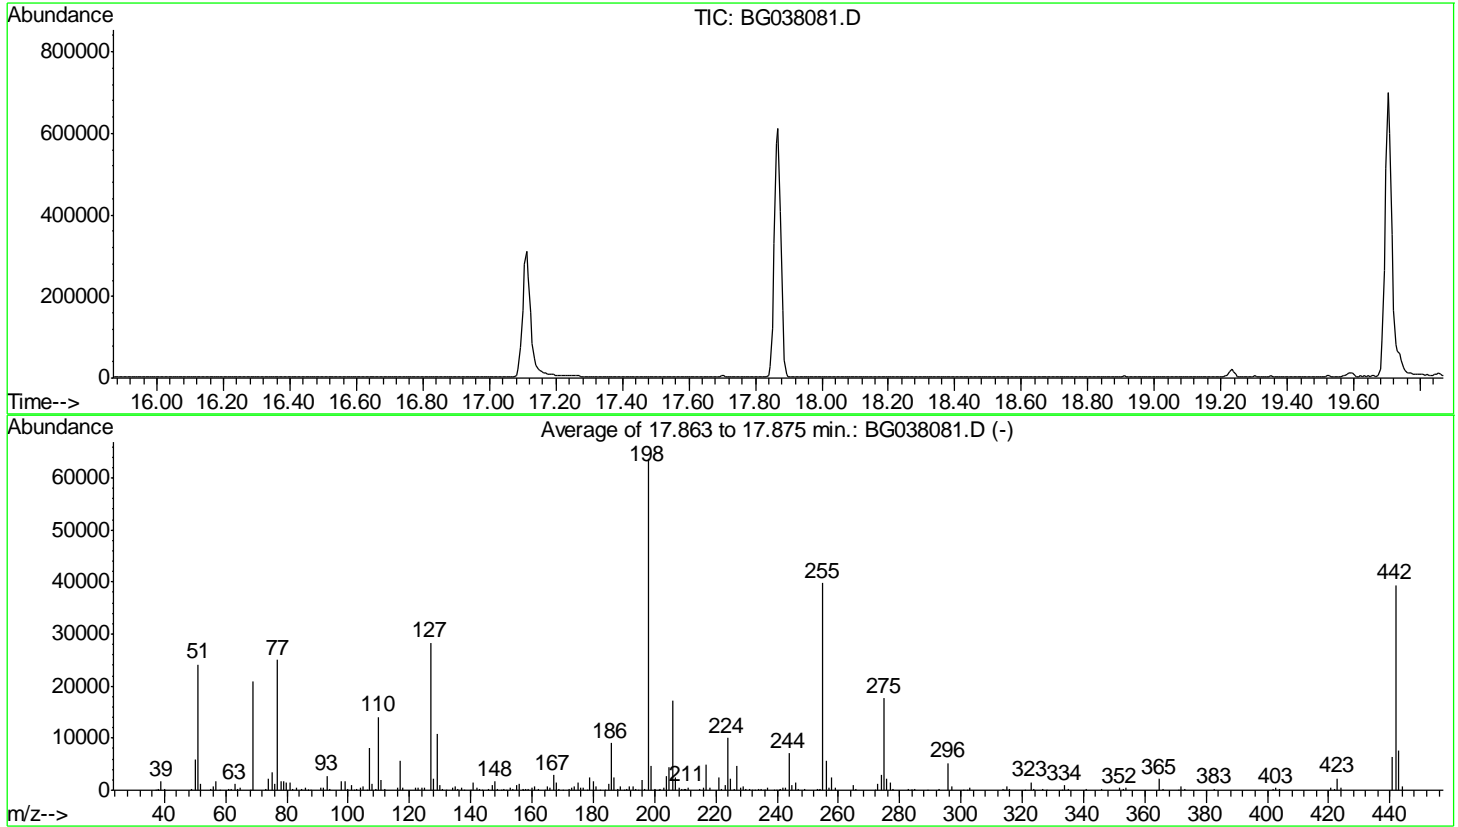

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	24160	PASS
68	69	0.00	2	0.6	127	PASS
69	198	0.00	100	32.9	20955	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	28330	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63701	PASS
199	198	5	9	7.2	4573	PASS
275	198	10	60	27.7	17656	PASS
365	198	1	100	3.4	2174	PASS
441	198	0.01	100	10.2	6498	PASS
442	198	50	100	61.8	39392	PASS
443	442	15	24	19.6	7732	PASS