


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112018\
 Data File : BG038099.D
 Acq On : 21 Nov 2018 1:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

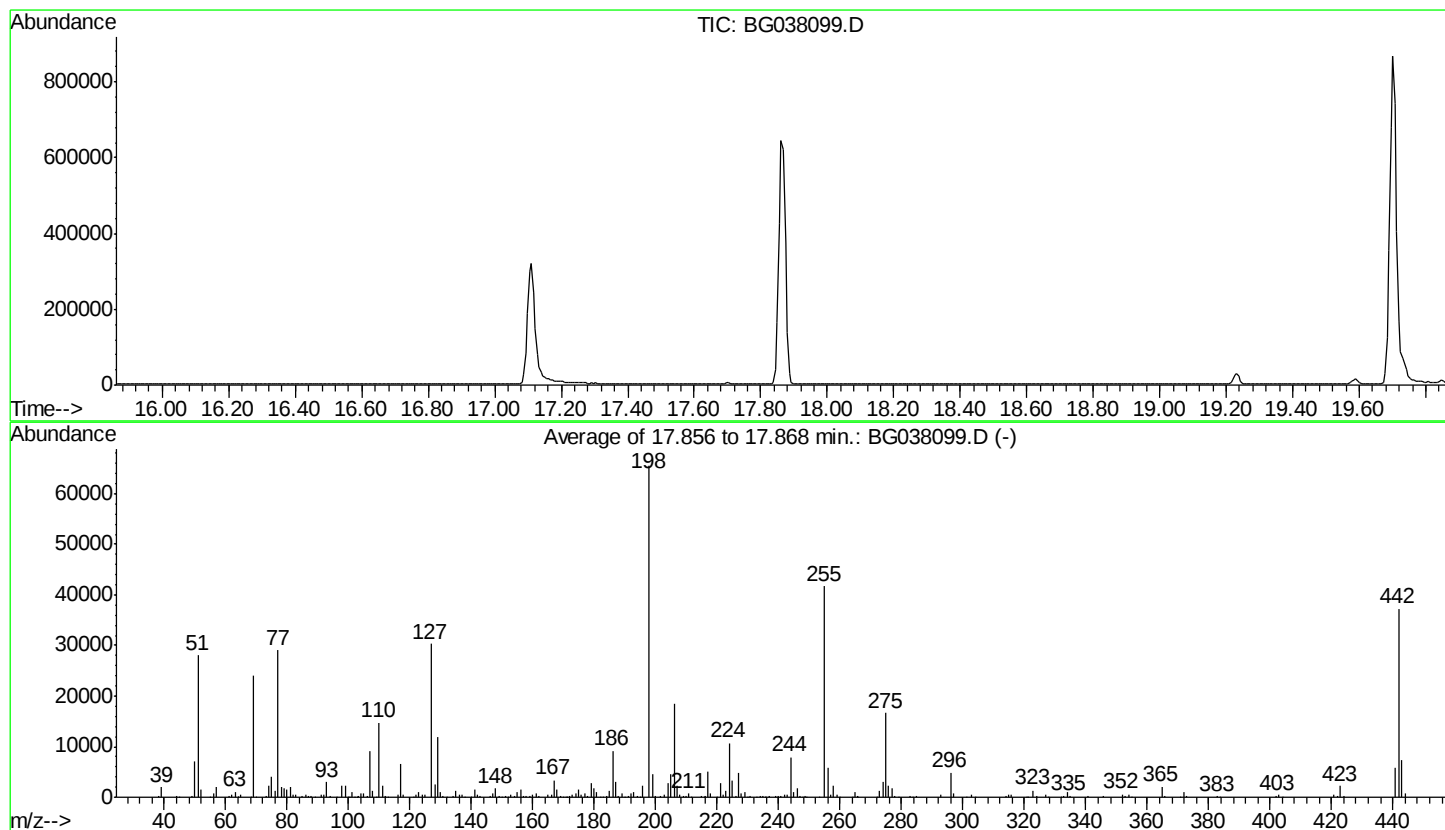

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	28045	PASS
68	69	0.00	2	0.5	116	PASS
69	198	0.00	100	36.8	24109	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	46.3	30362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65554	PASS
199	198	5	9	7.0	4609	PASS
275	198	10	60	25.5	16701	PASS
365	198	1	100	3.2	2096	PASS
441	198	0.01	100	9.0	5916	PASS
442	198	50	100	56.8	37261	PASS
443	442	15	24	19.4	7234	PASS