
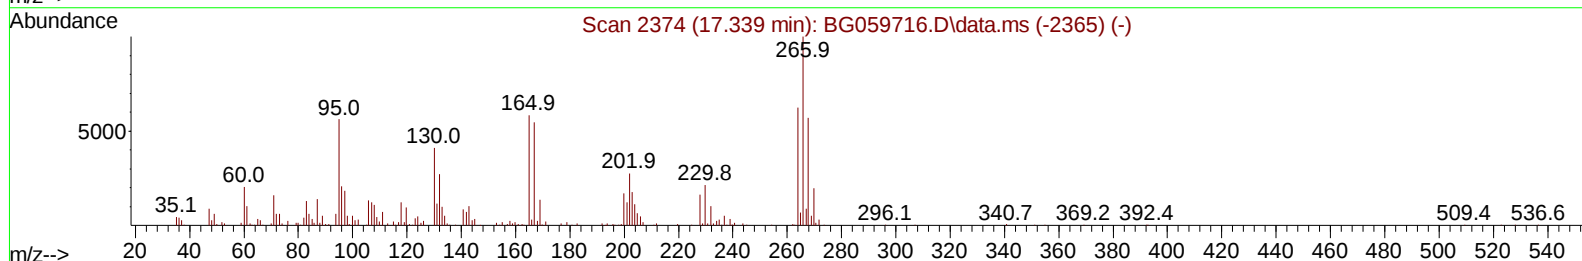
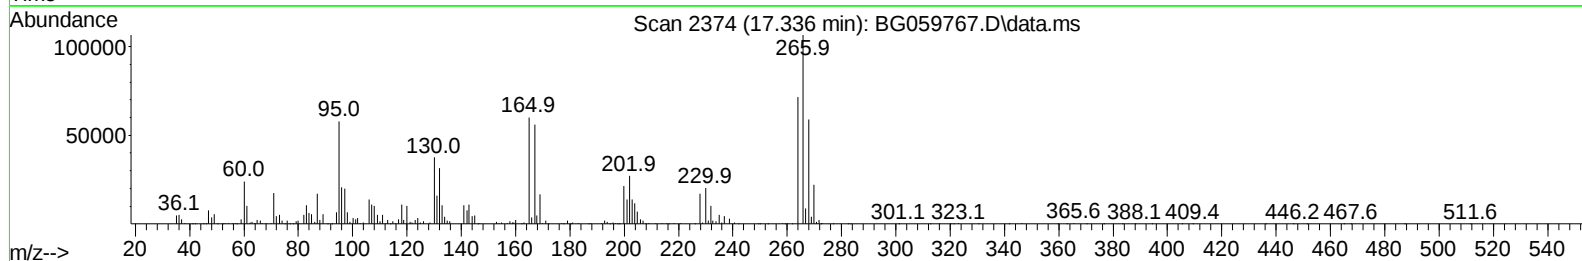


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112023\
Data File : BG059767.D
Acq On : 20 Nov 2023 13:40
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 02:17:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

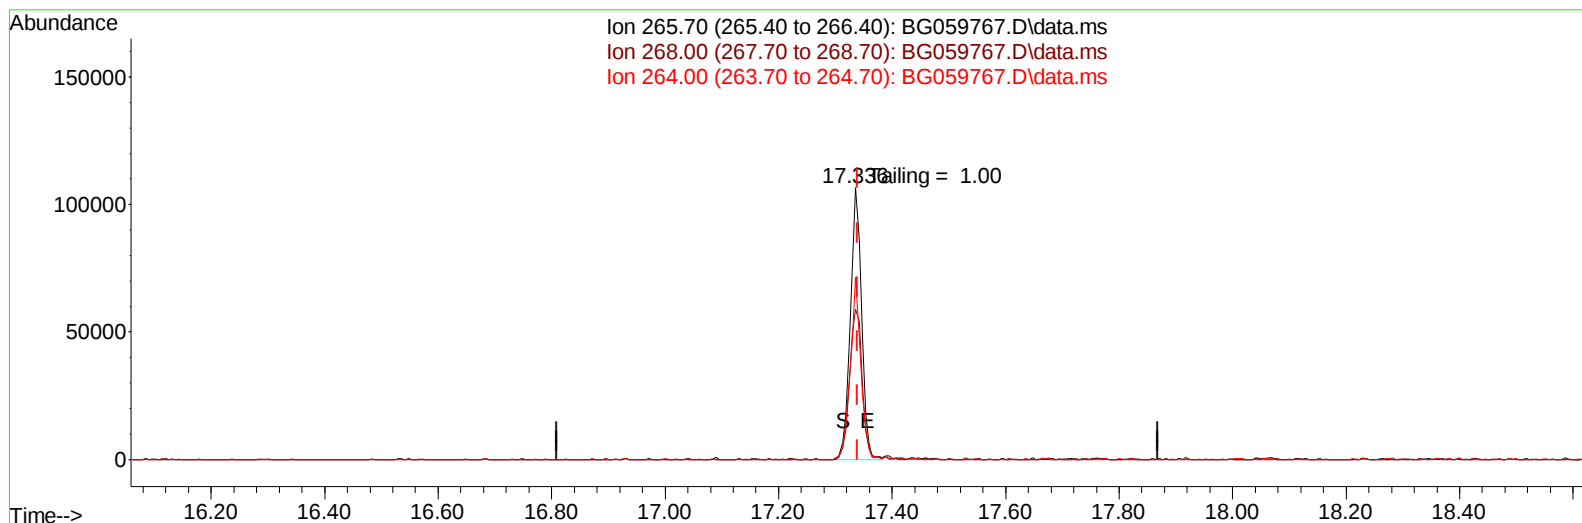

TIC: BG059767.D\data.ms




(70) Pentachlorophenol (C)

17.336min (-0.003) 239519.70 ng

response 144747

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	55.42
264.00	62.30	67.20
0.00	0.00	0.00

Quant Time: Nov 21 02:17:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

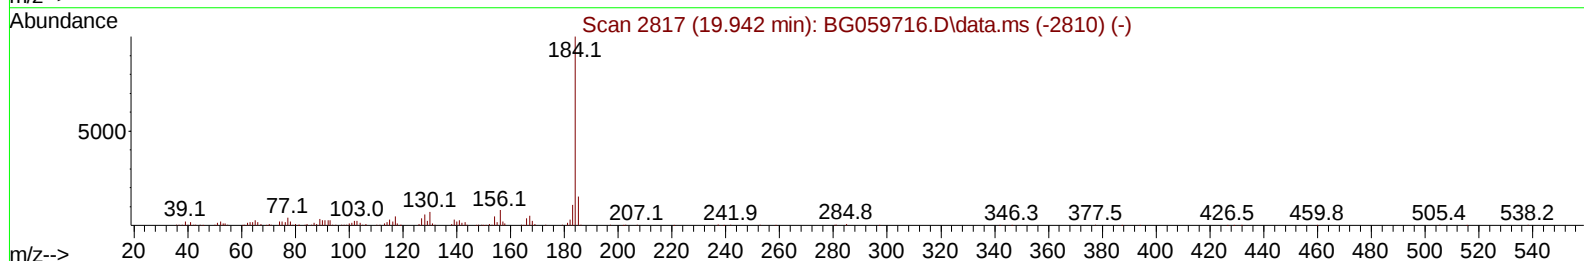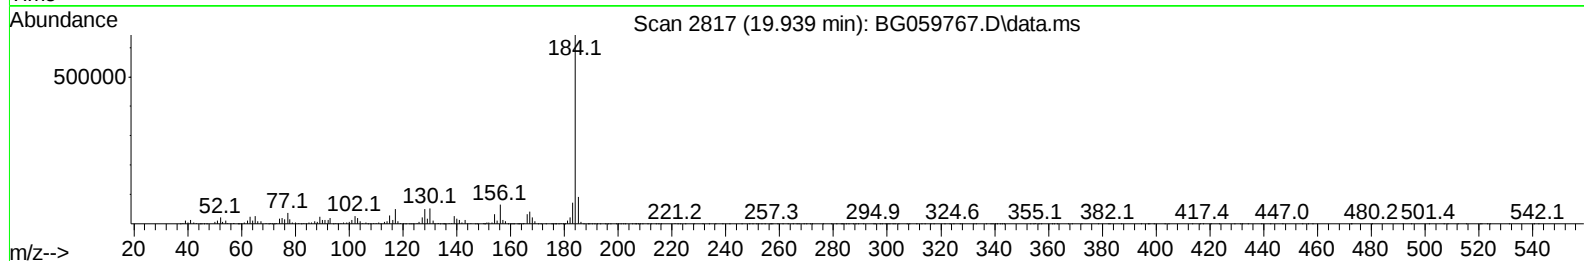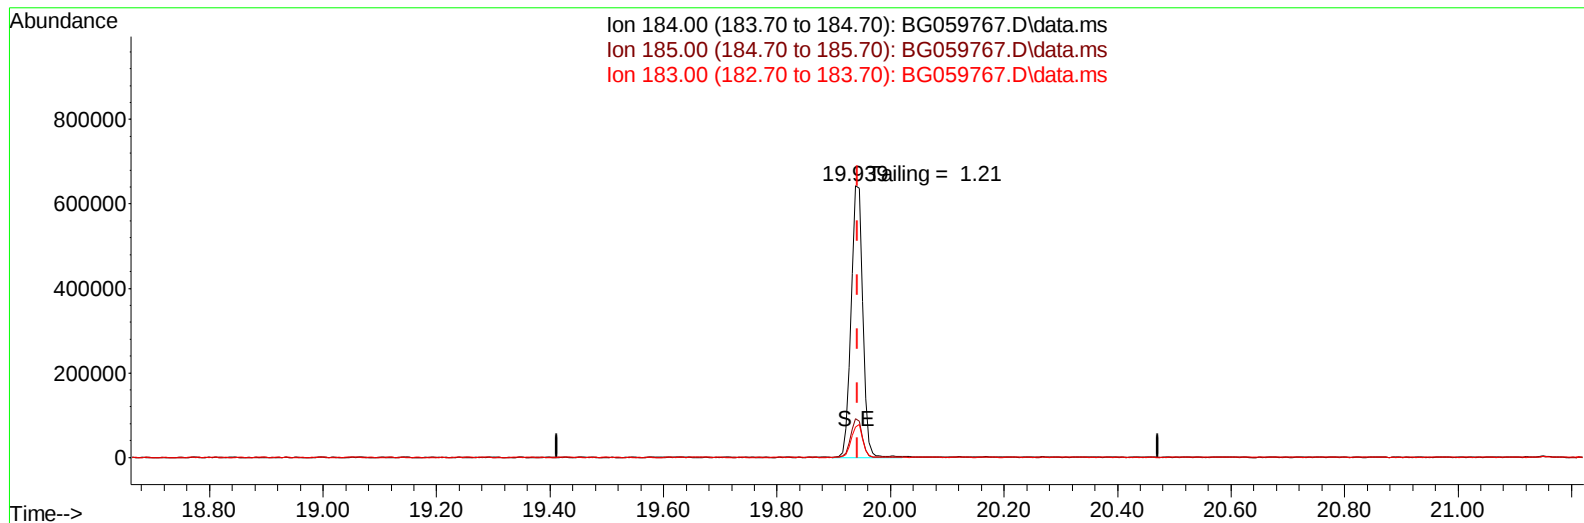

TIC: BG059767.D\data.ms

(77) Benzidine

19.939min (-0.003) 56734.26 ng

response **909550**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.37
183.00	11.00	11.23
0.00	0.00	0.00