
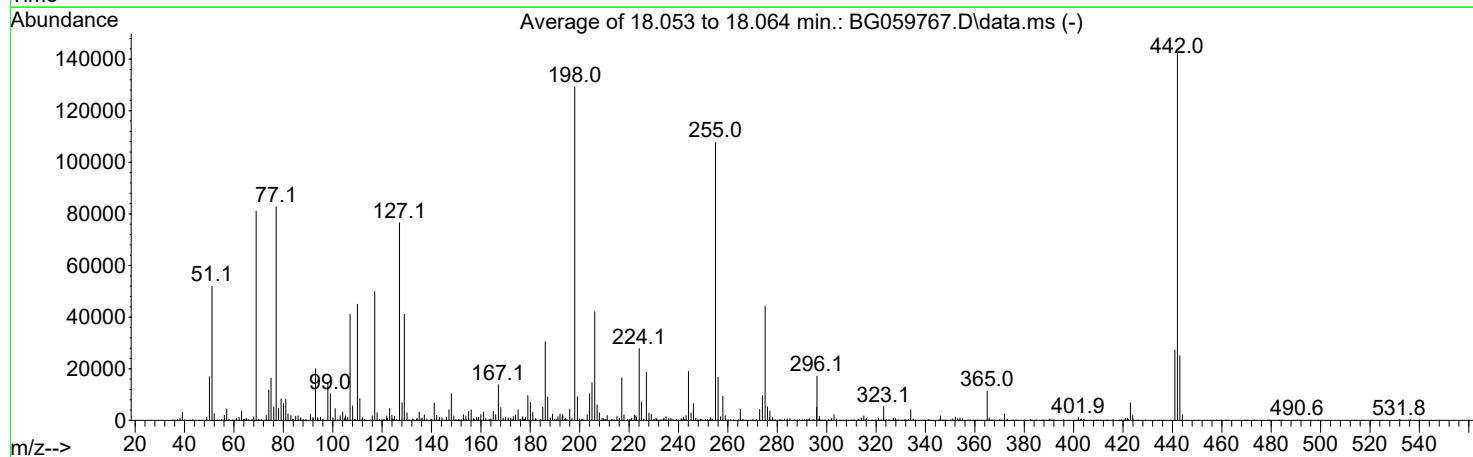


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112023\
Data File : BG059767.D
Acq On : 20 Nov 2023 13:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 17 01:51:38 2023

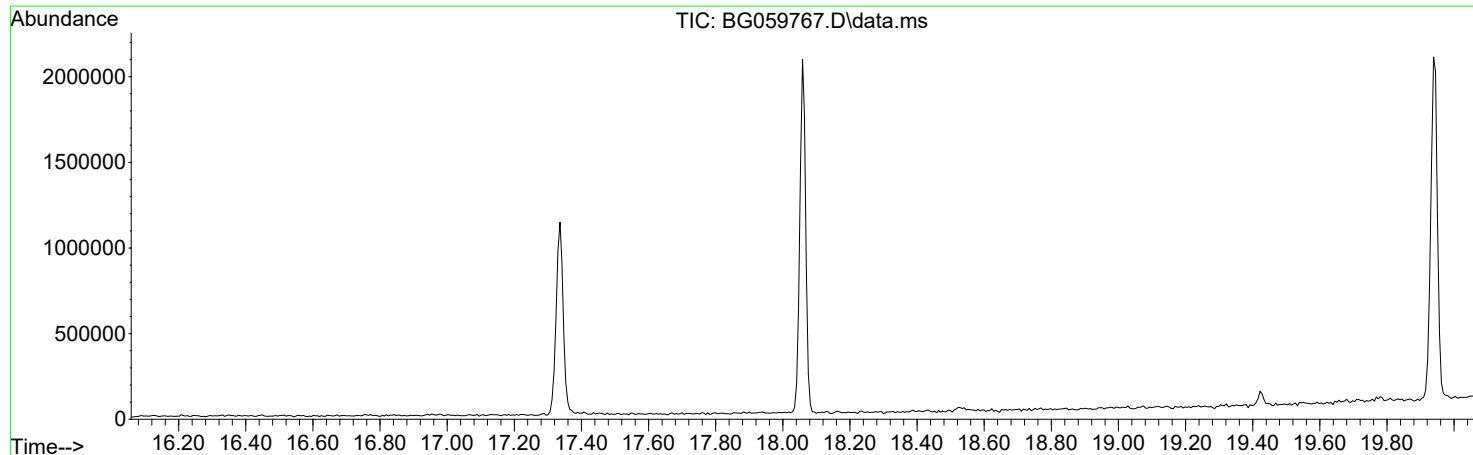

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	51941	PASS
68	69	0.00	2	1.7	1361	PASS
69	198	0.00	100	62.8	81139	PASS
70	69	0.00	2	0.6	457	PASS
127	198	10	80	59.3	76607	PASS
197	198	0.00	2	0.7	871	PASS
198	198	100	100	100.0	129264	PASS
199	198	5	9	7.1	9202	PASS
275	198	10	60	34.3	44307	PASS
365	198	1	100	8.7	11280	PASS
441	198	0.01	100	21.1	27261	PASS
442	442	50	100	100.0	142571	PASS
443	442	15	24	17.6	25085	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/20/2023	BNA_G	<u>BG059767.D</u>
Compound Name	Response	Retention Time
DDT	335894	21.149
DDD	12500	20.691
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12500	348394	3.59

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112023\
Data File : BG059767.D
Acq On : 20 Nov 2023 13:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 21 02:17:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

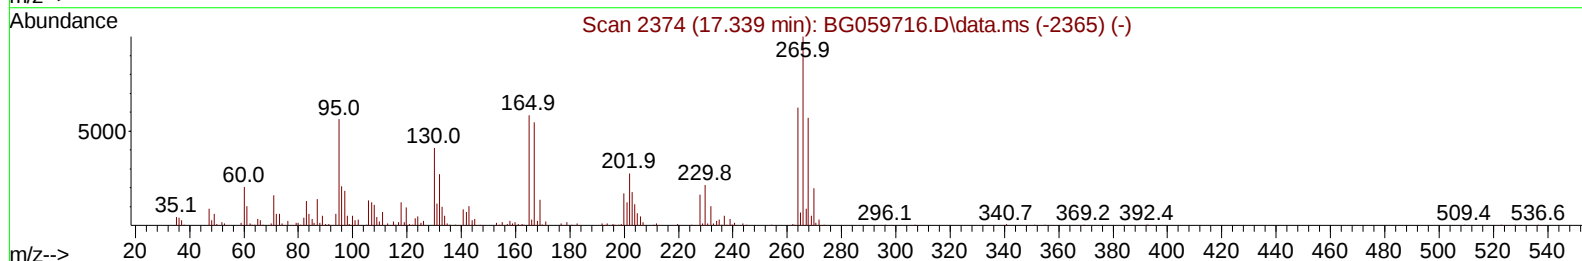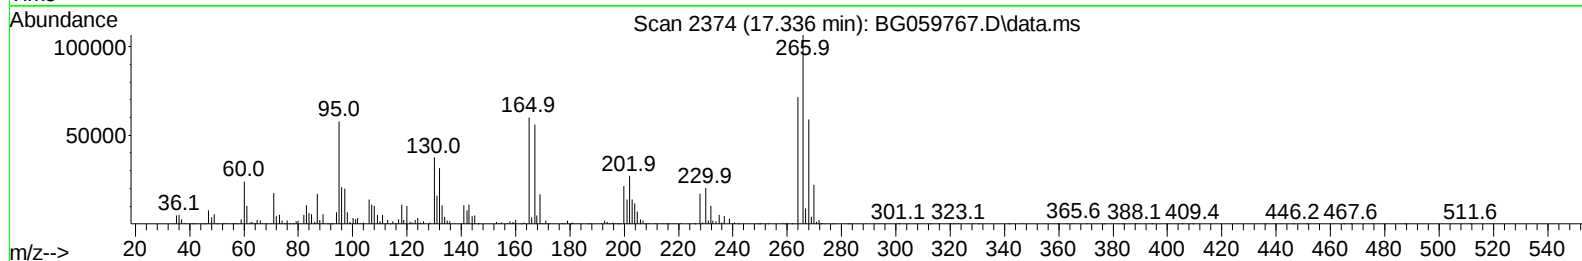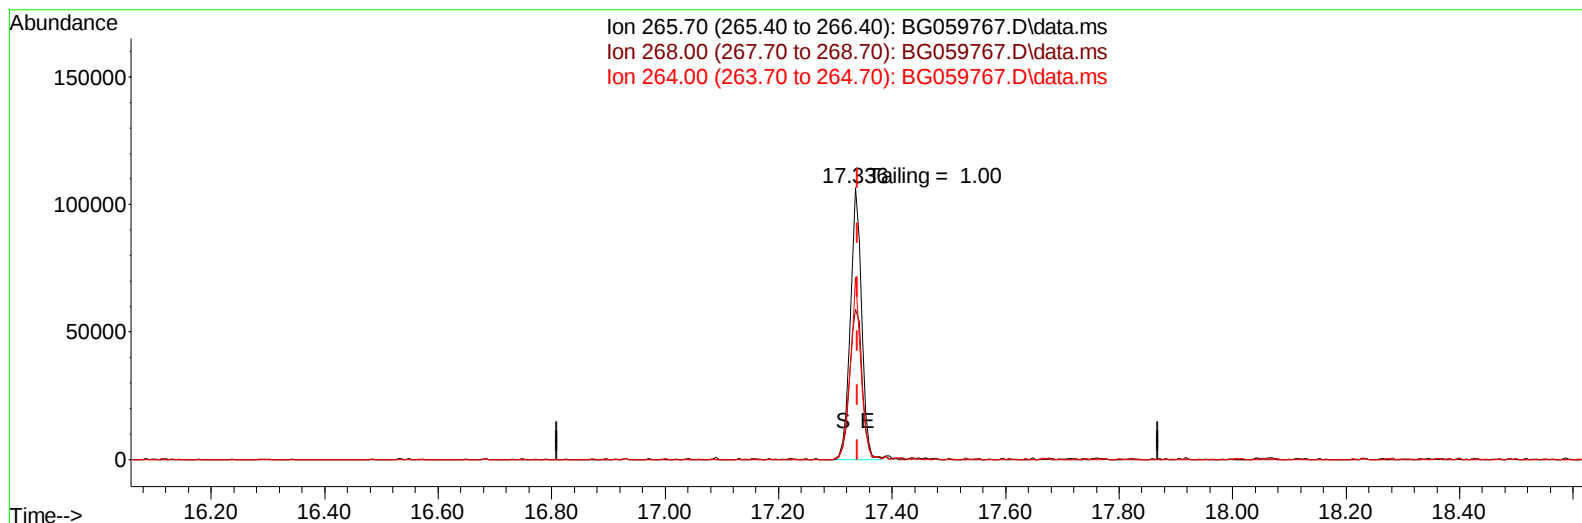

TIC: BG059767.D\data.ms

(70) Pentachlorophenol (C)

17.336min (-0.003) 239519.70 ng




response 144747

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	55.42
264.00	62.30	67.20
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112023\  
Data File : BG059767.D  
Acq On    : 20 Nov 2023 13:40  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 21 02:17:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

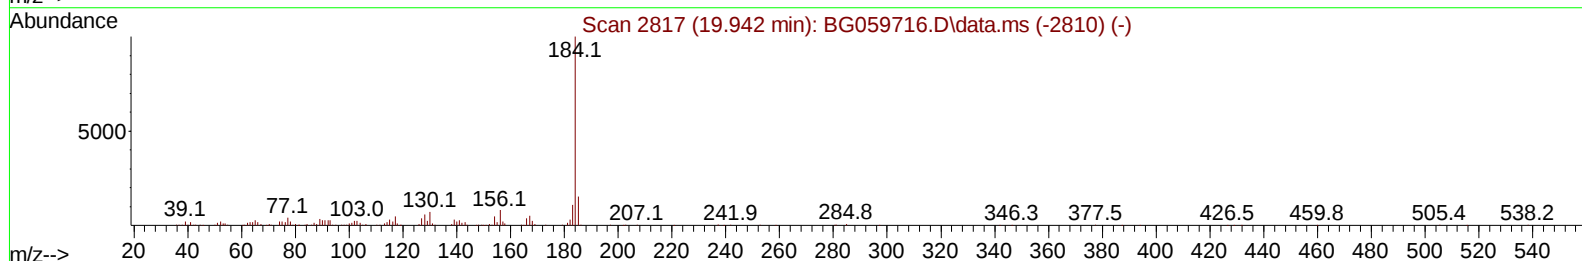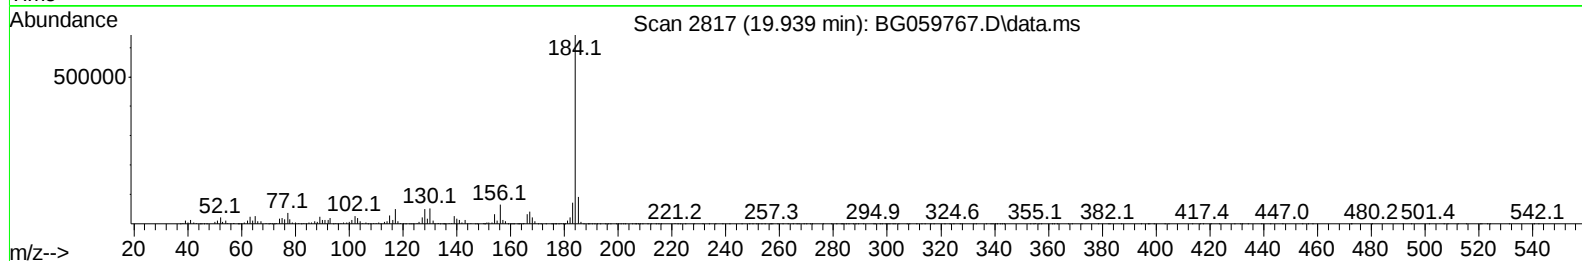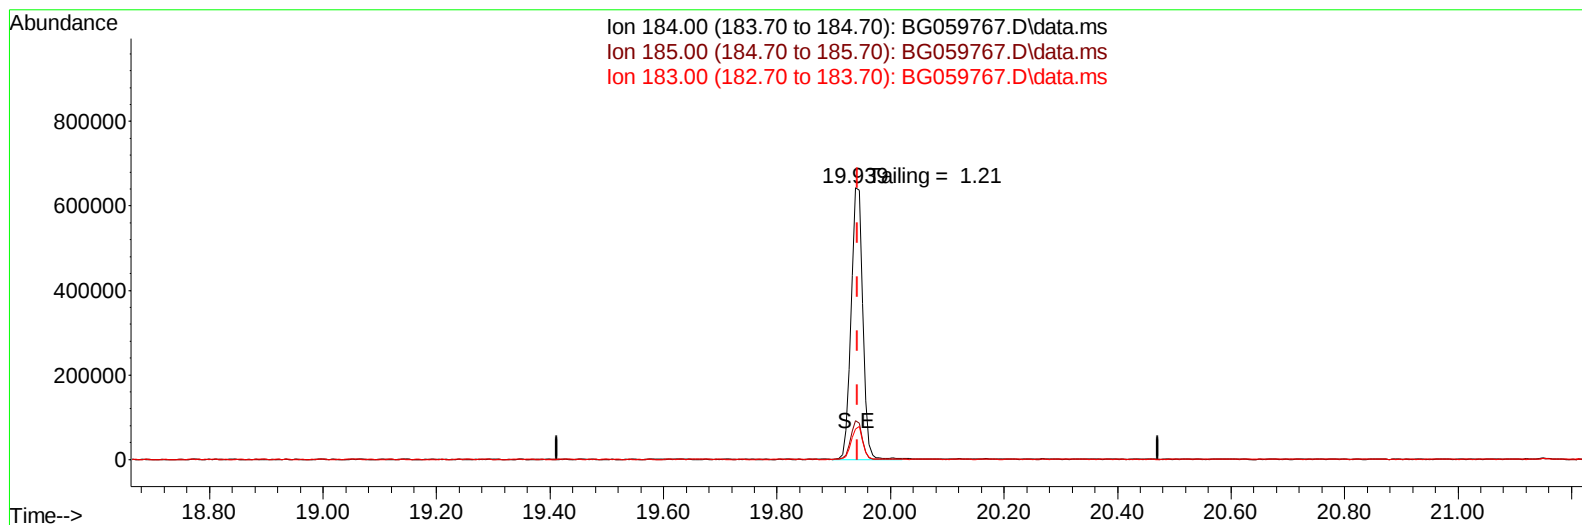

TIC: BG059767.D\data.ms

(77) **Benzidine**

19.939min (-0.003) 56734.26 ng

response **909550**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.37
183.00	11.00	11.23
0.00	0.00	0.00