


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112025\
Data File : BG064826.D
Acq On : 20 Nov 2025 9:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

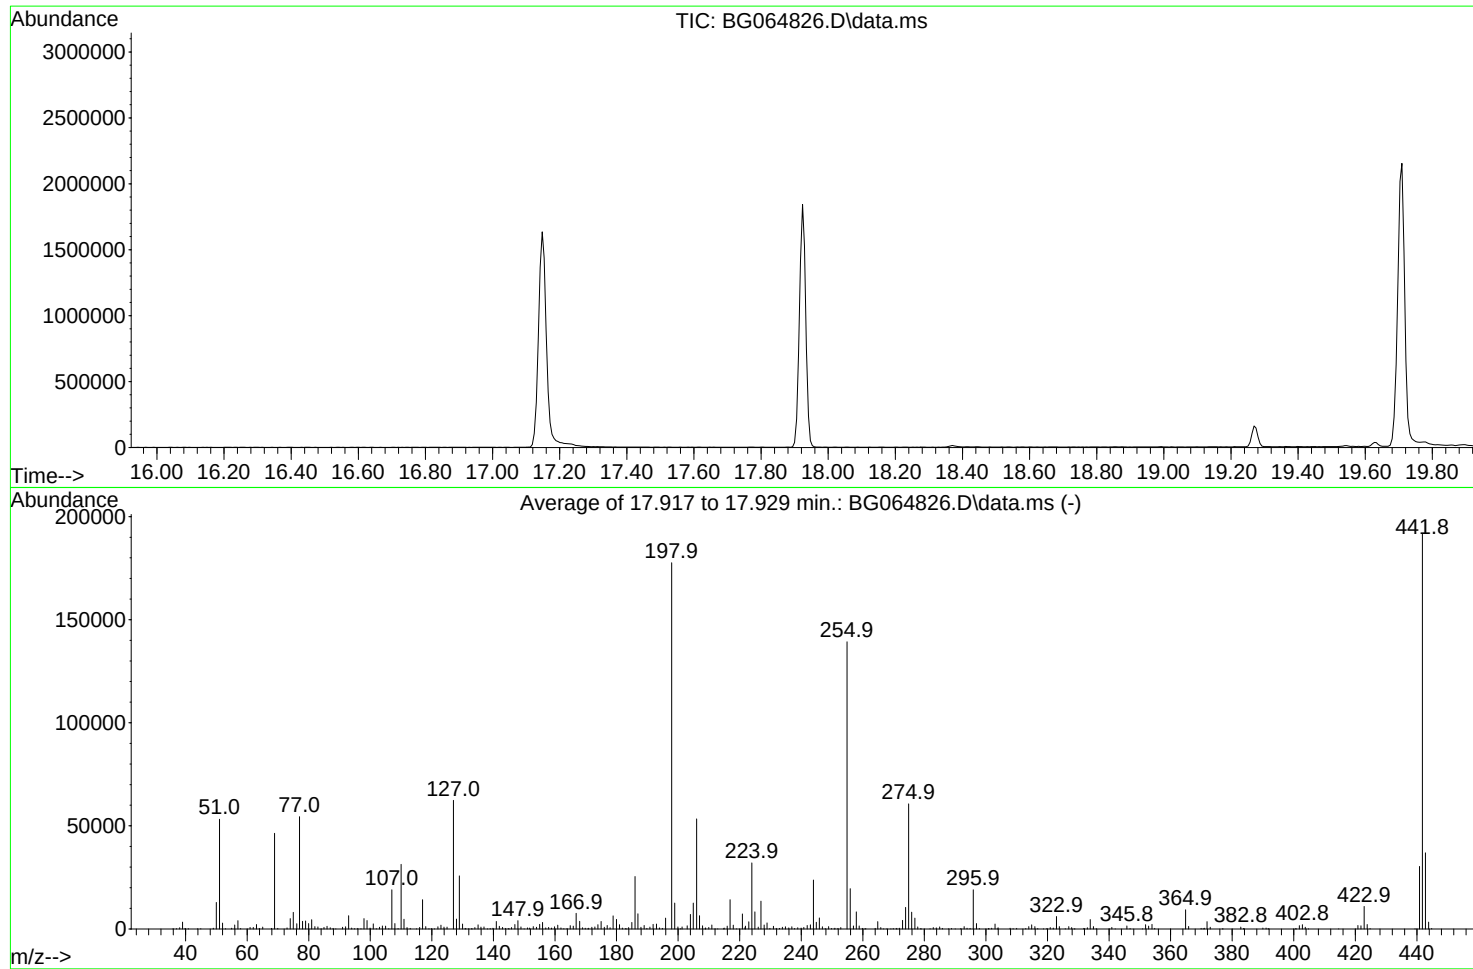

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.5	246	PASS
69	69	100	100	100.0	46357	PASS
70	69	0.00	2	0.6	258	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177643	PASS
199	198	5	9	7.0	12504	PASS
365	198	1	100	5.2	9285	PASS
441	443	0.01	150	82.2	30341	PASS
442	442	100	100	100.0	191531	PASS
443	442	15	24	19.3	36925	PASS

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112025\
 Data File : BG064826.D
 Acq On : 20 Nov 2025 9:18
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




Quant Time: Nov 20 09:55:09 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 12 17:10:56 2025
 Response via : Initial Calibration



Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112025\
Data File : BG064826.D
Acq On : 20 Nov 2025 9:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 20 09:55:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

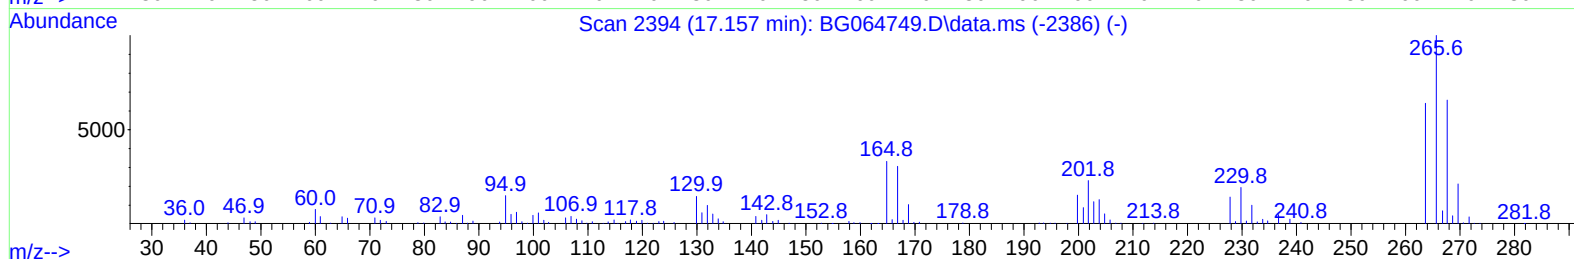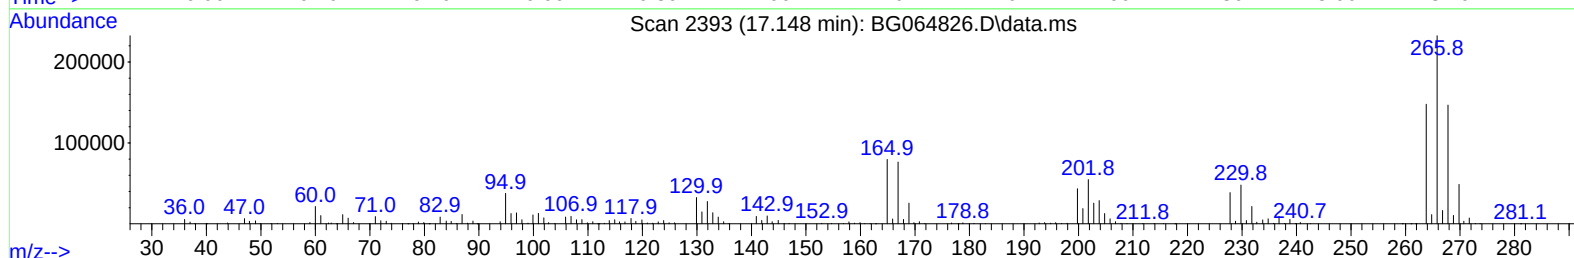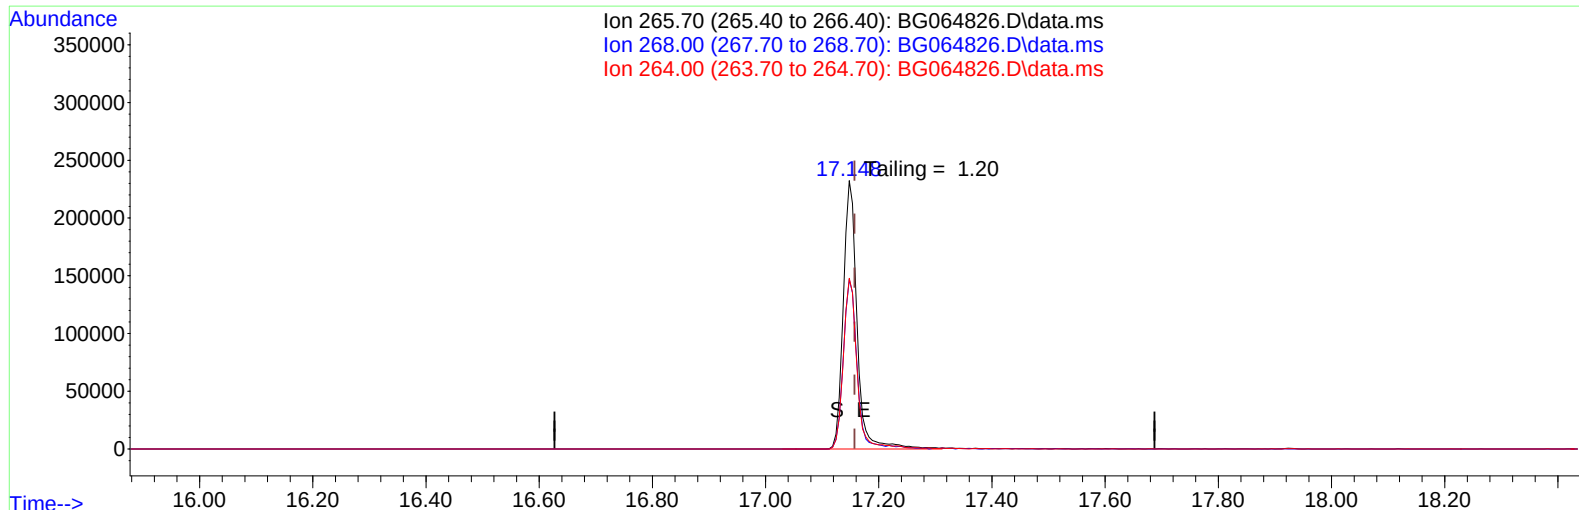

TIC: BG064826.D\data.ms

(70) Pentachlorophenol (C)

17.148min (-0.009) 274268.75 ng

response 397178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	63.18
264.00	64.00	63.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/20/2025	BNA_G	<u>BG064826.D</u>
Compound Name	Response	Retention Time
DDT	897918	20.937
DDD	22643	20.491
DDE	546	19.269
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23189	921107	2.52

Instrument :
BNA_G
ClientSampleId :
DFTPP