


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112118\
 Data File : BG038117.D
 Acq On : 21 Nov 2018 14:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

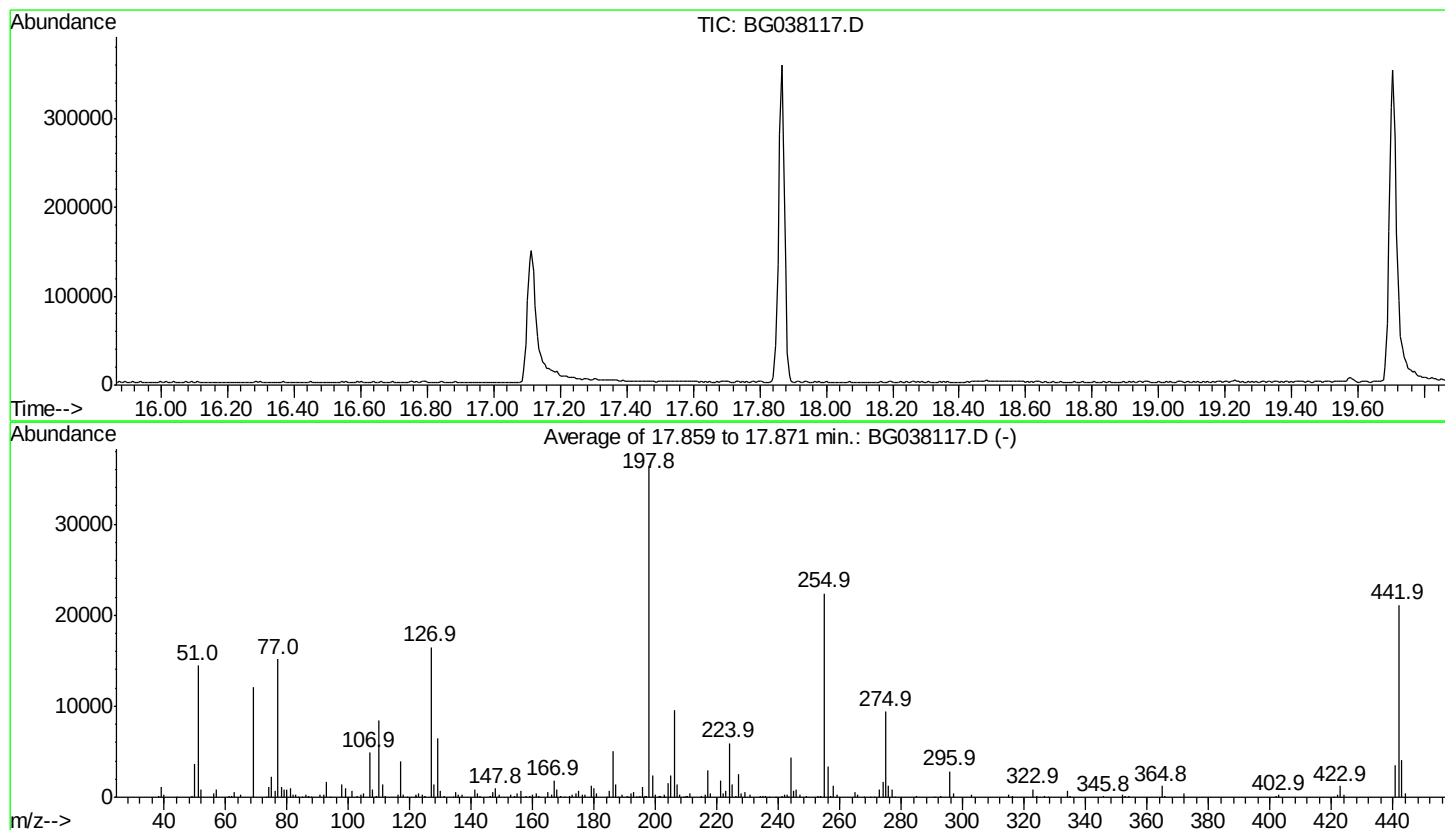

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	14472	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	12120	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	16506	PASS
197	198	0.00	2	0.5	177	PASS
198	198	100	100	100.0	36426	PASS
199	198	5	9	6.6	2393	PASS
275	198	10	60	25.8	9398	PASS
365	198	1	100	3.3	1216	PASS
441	198	0.01	100	9.6	3503	PASS
442	198	50	100	58.0	21119	PASS
443	442	15	24	19.6	4137	PASS