
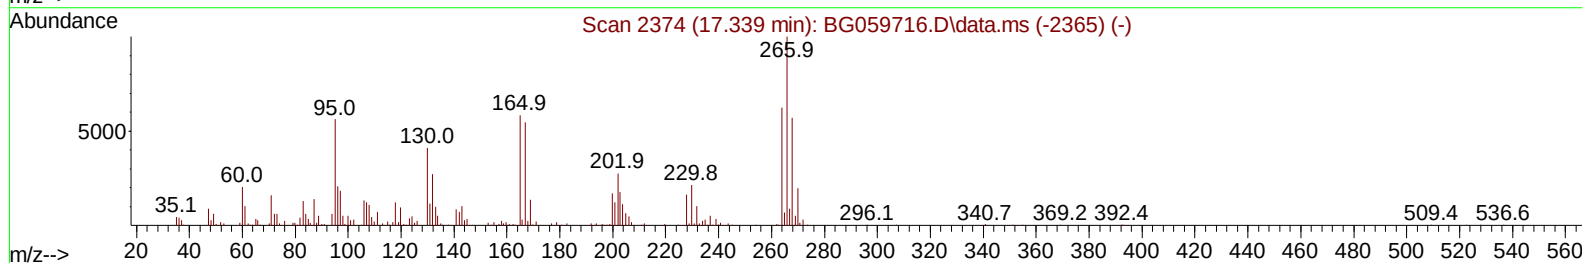
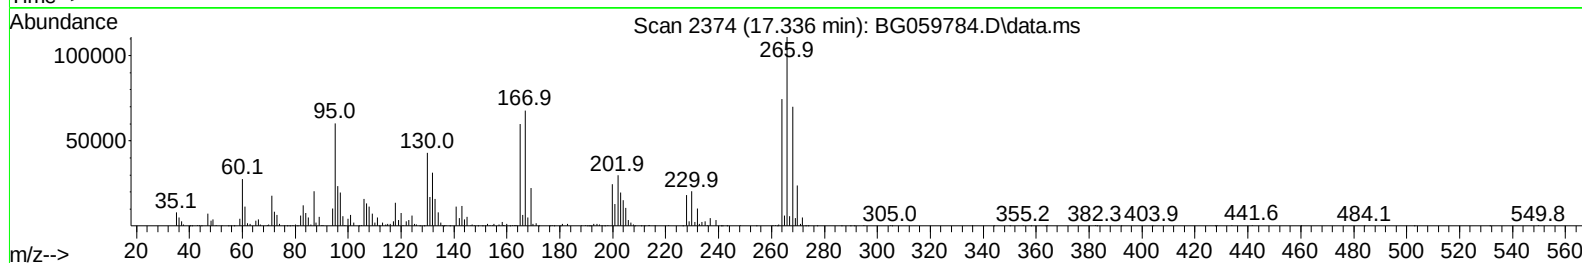


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
Data File : BG059784.D
Acq On : 21 Nov 2023 9:06
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 03:54:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

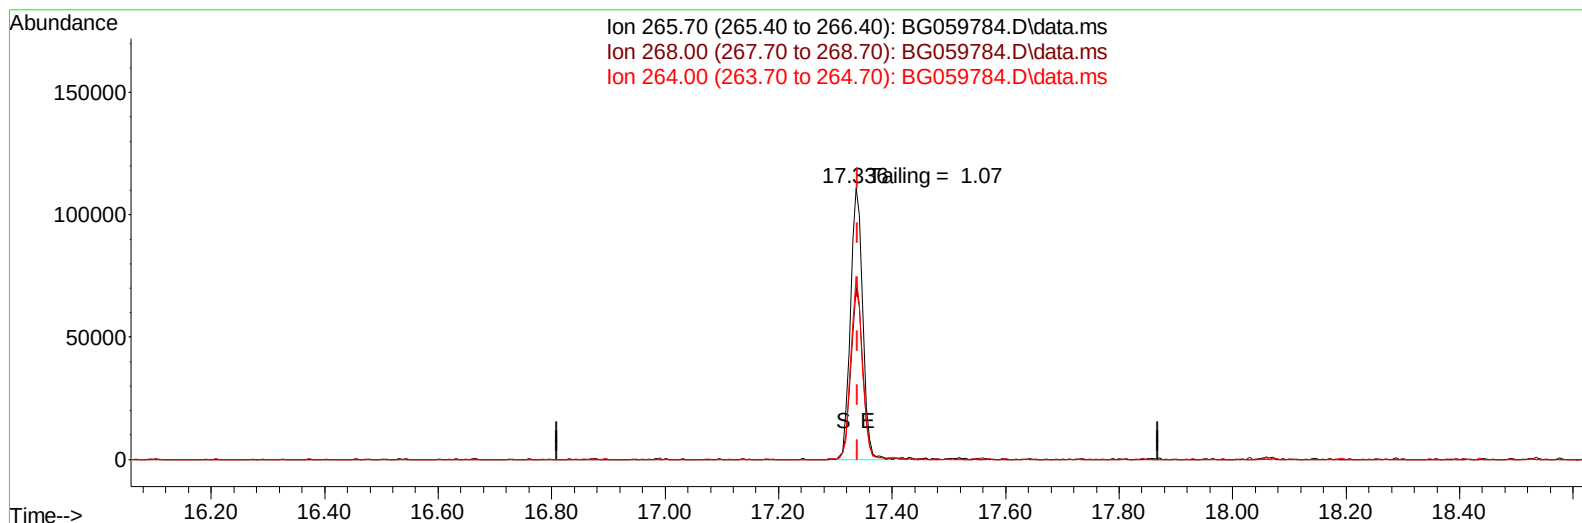



TIC: BG059784.D\data.ms

(70) Pentachlorophenol (C)

17.336min (-0.002) 333157.78 ng

response 165655

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	63.12
264.00	62.30	67.25
0.00	0.00	0.00

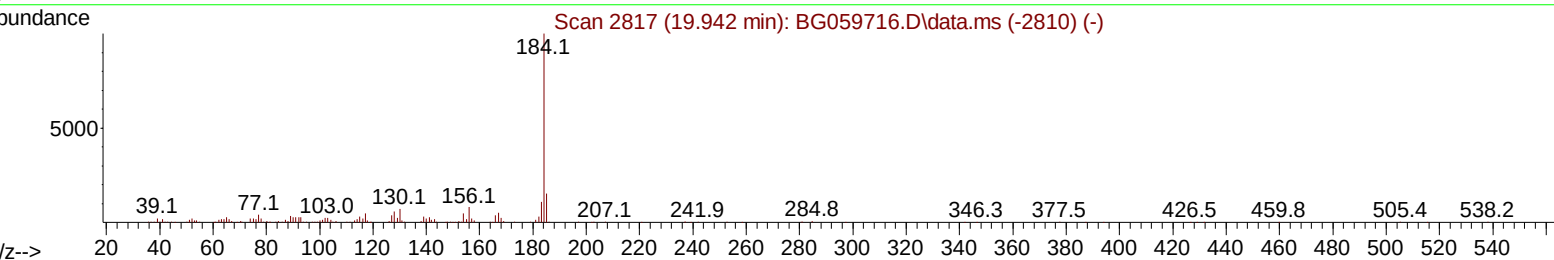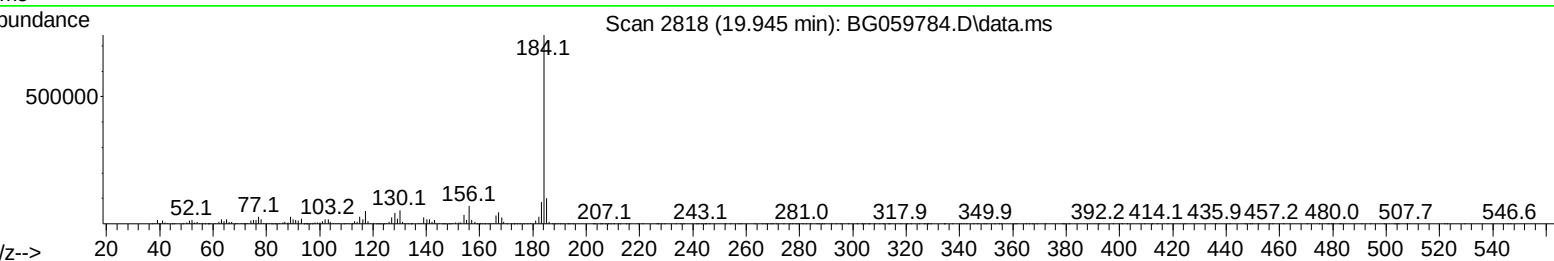

TIC: BG059784.D\data.ms

19.945min (+ 0.004) 185179.03 ng

response **1016176**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.52
183.00	11.00	11.40
0.00	0.00	0.00