
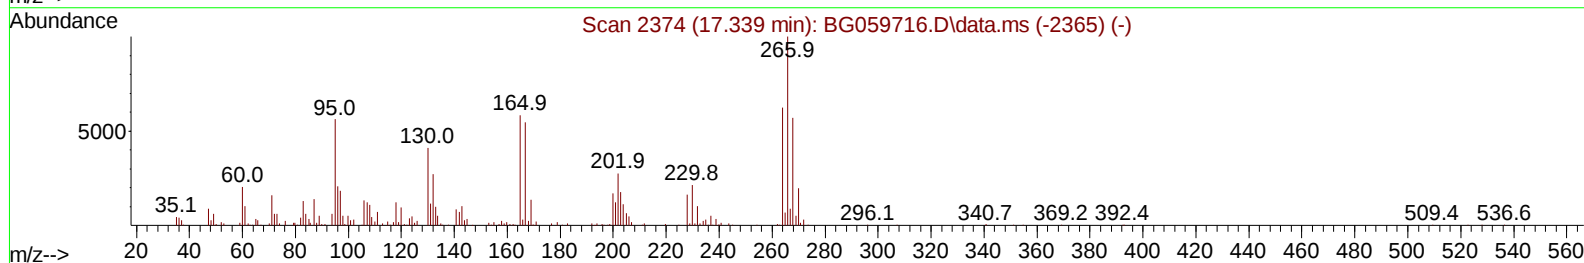
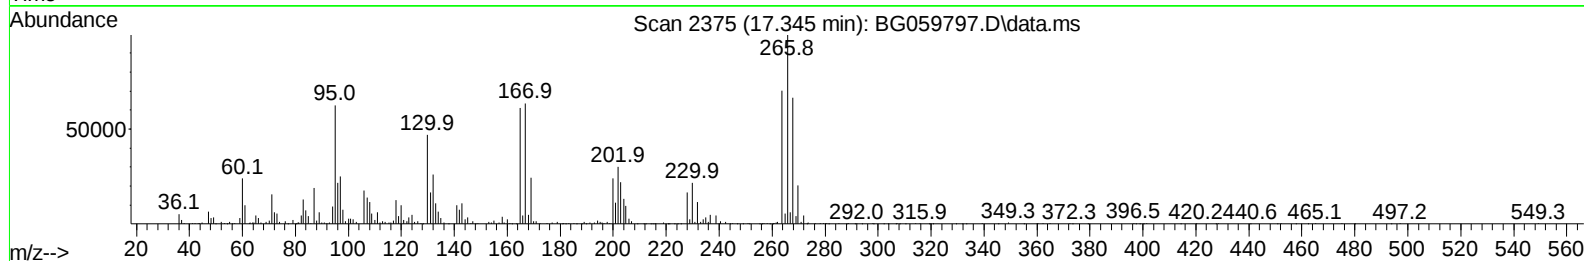


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
Data File : BG059797.D
Acq On : 21 Nov 2023 18:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 01:55:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

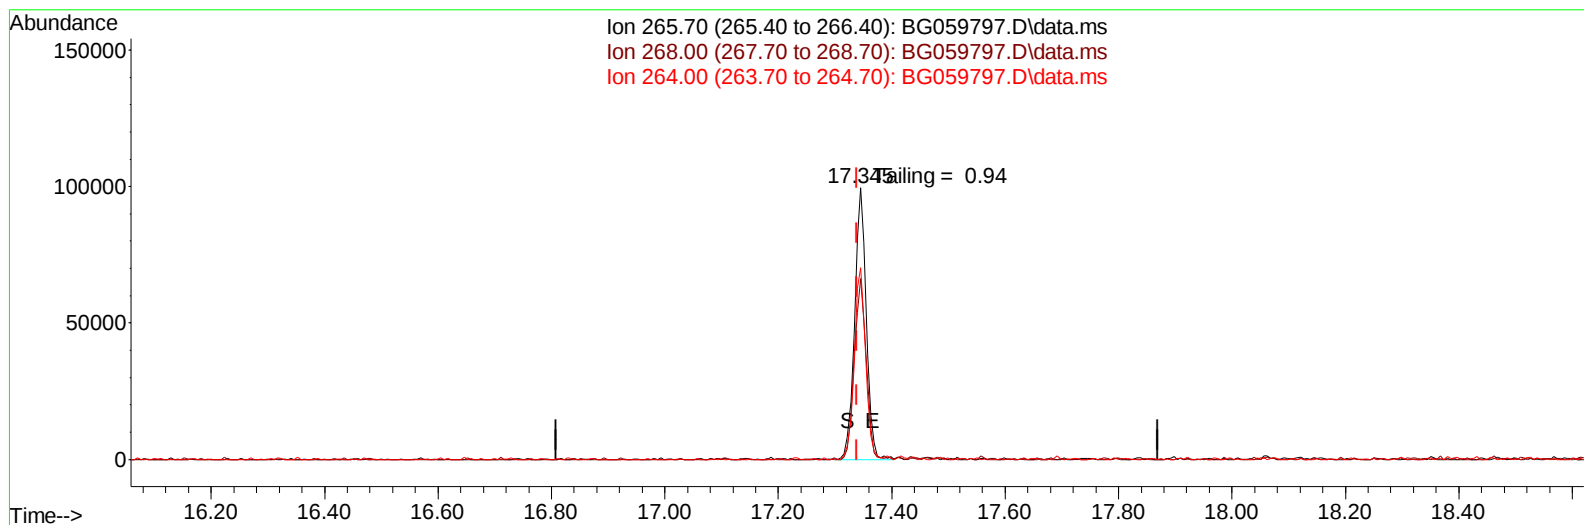

TIC: BG059797.D\data.ms

(70) Pentachlorophenol (C)




17.345min (+ 0.007) 27321.34 ng

response 141283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	66.68
264.00	62.30	70.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
Data File : BG059797.D
Acq On : 21 Nov 2023 18:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 01:55:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

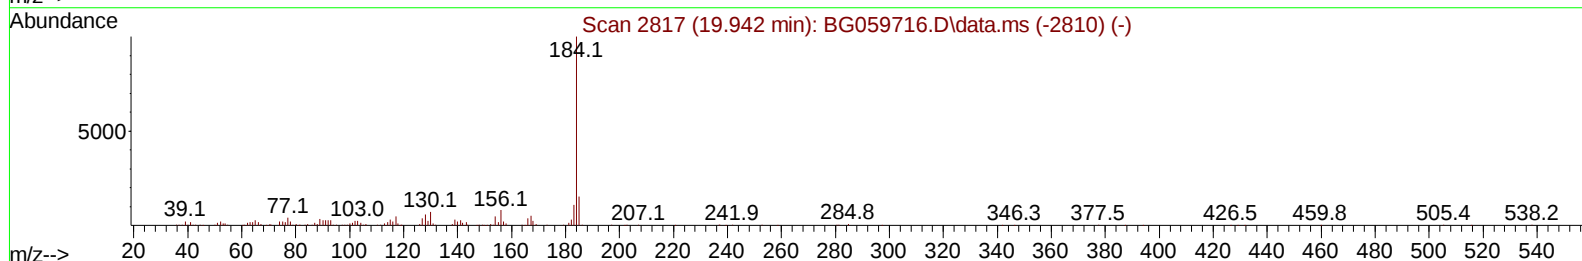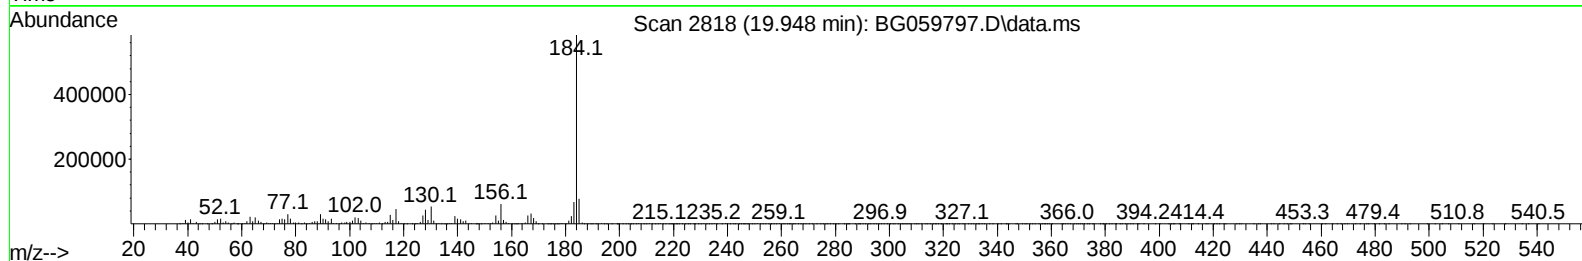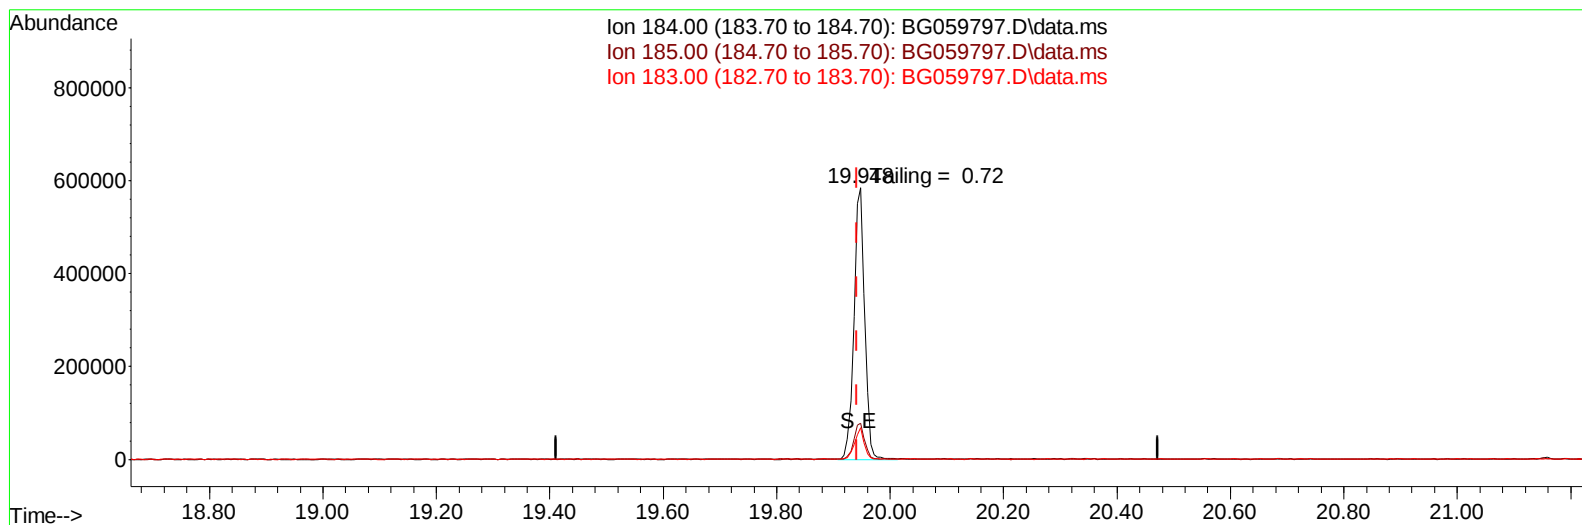

TIC: BG059797.D\data.ms

(77) Benzidine**19.948min (+ 0.007) 17422.40 ng****response 769984**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.41
183.00	11.00	11.70
0.00	0.00	0.00