
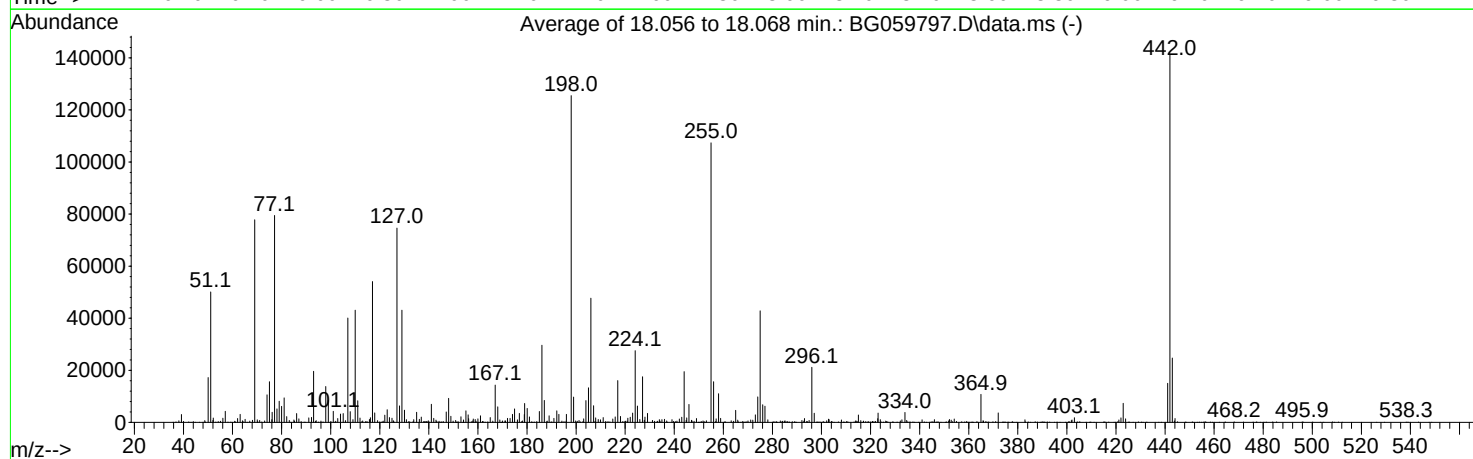


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
 Data File : BG059797.D
 Acq On : 21 Nov 2023 18:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 01:51:38 2023

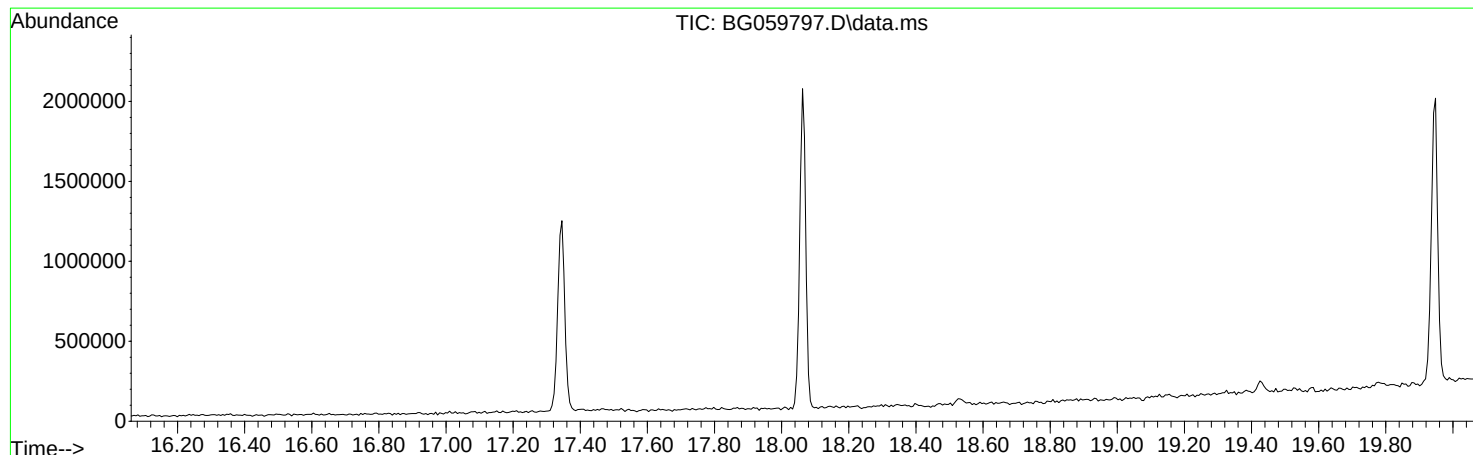




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	50077	PASS
68	69	0.00	2	1.0	786	PASS
69	198	0.00	100	62.0	77813	PASS
70	69	0.00	2	1.3	984	PASS
127	198	10	80	59.5	74624	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125509	PASS
199	198	5	9	7.7	9696	PASS
275	198	10	60	34.1	42825	PASS
365	198	1	100	8.6	10753	PASS
441	198	0.01	100	11.9	14994	PASS
442	442	50	100	100.0	141291	PASS
443	442	15	24	17.5	24729	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
Data File : BG059797.D
Acq On : 21 Nov 2023 18:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 01:55:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

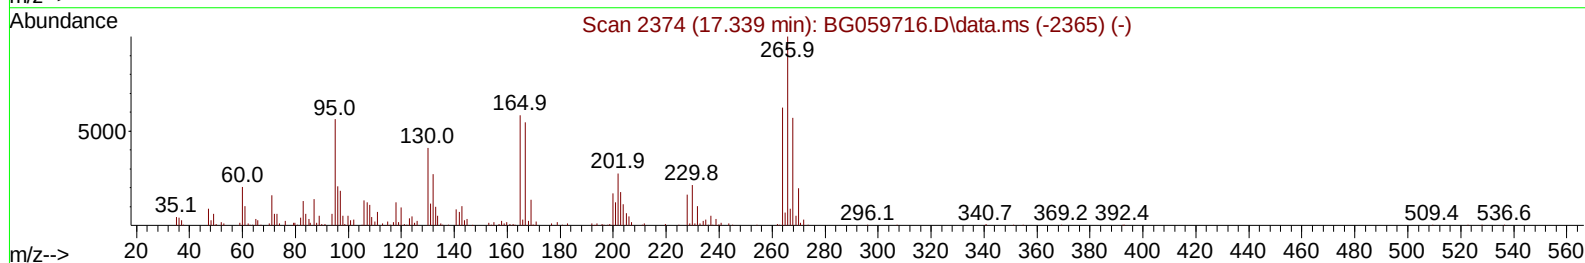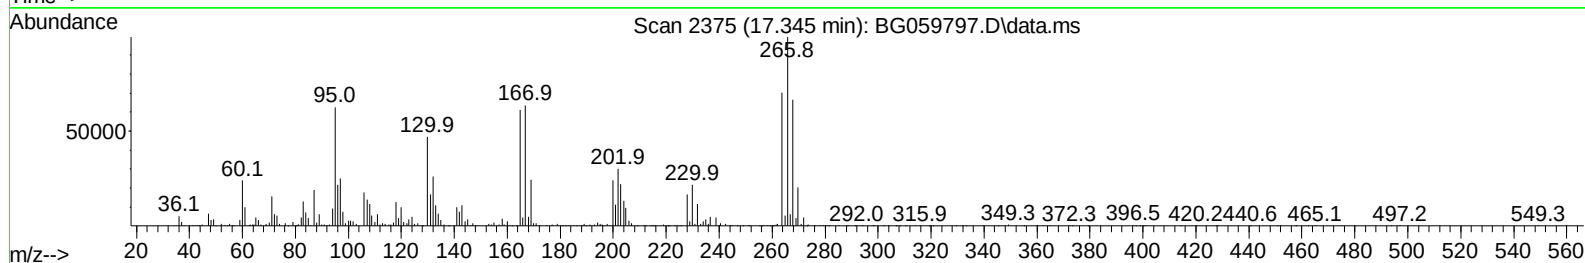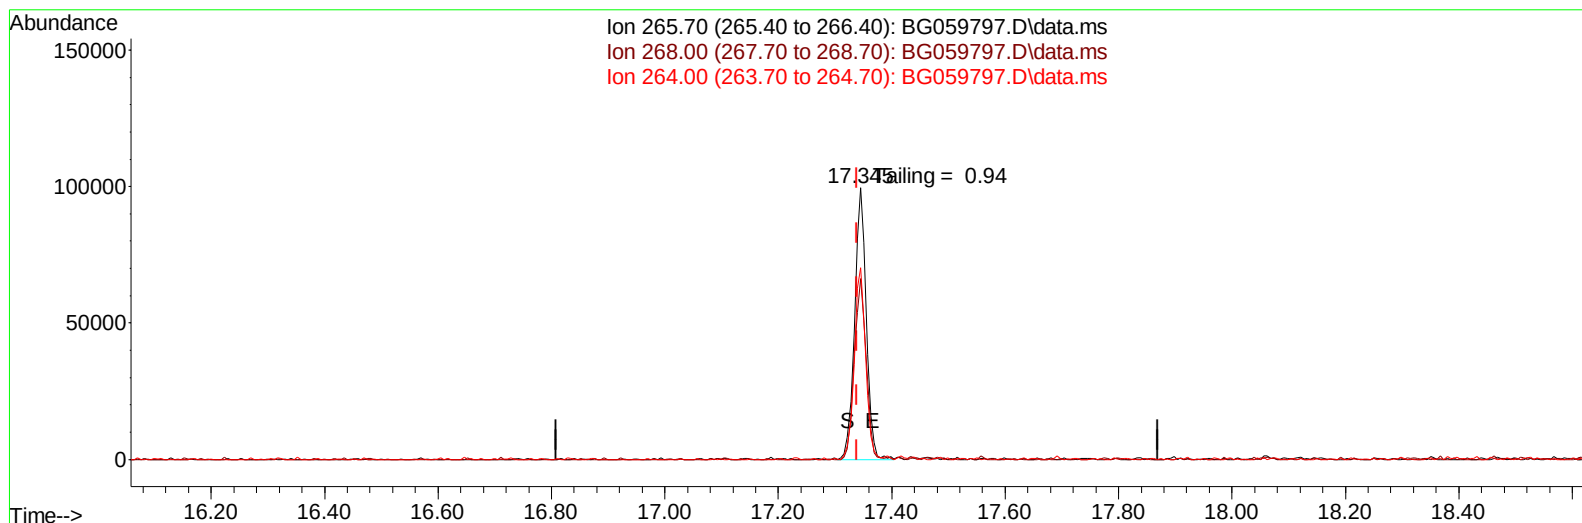

TIC: BG059797.D\data.ms

(70) Pentachlorophenol (C)

17.345min (+ 0.007) 27321.34 ng




response 141283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.10	66.68
264.00	62.30	70.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112123\
Data File : BG059797.D
Acq On : 21 Nov 2023 18:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 01:55:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 01:51:38 2023
Response via : Initial Calibration

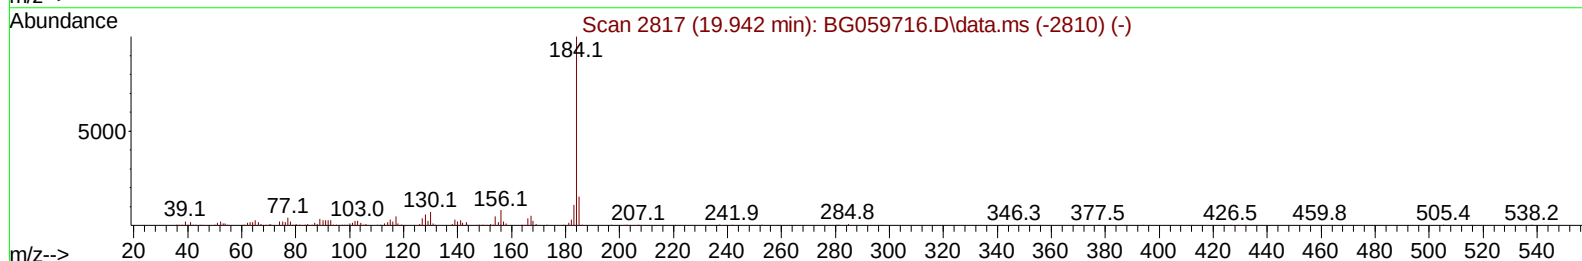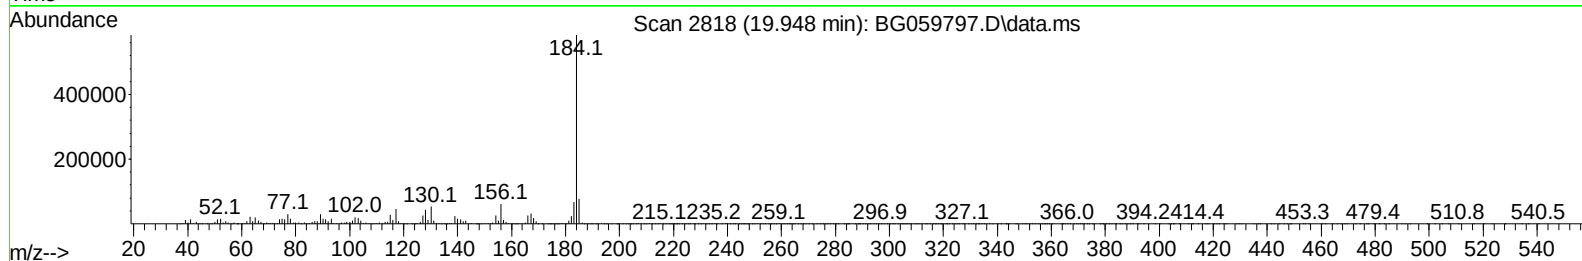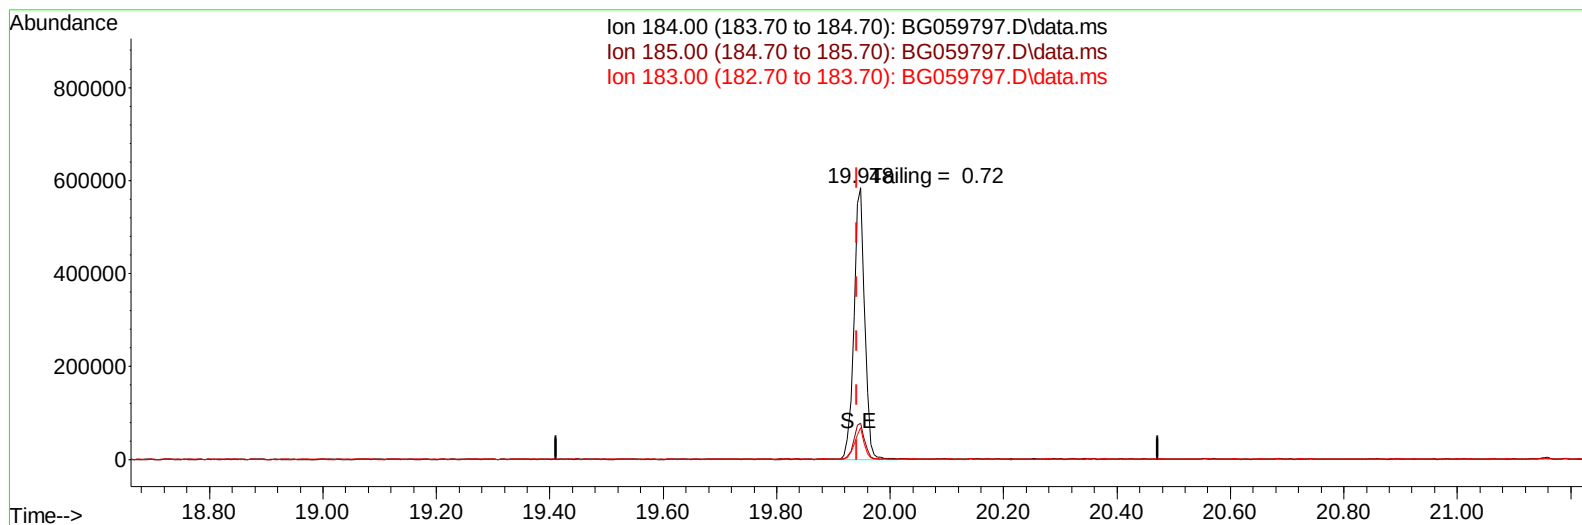

TIC: BG059797.D\data.ms

(77) Benzidine

19.948min (+ 0.007) 17422.40 ng

response 769984

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.41
183.00	11.00	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2023	BNA_G	<u>BG059797.D</u>
Compound Name	Response	Retention Time
DDT	316507	21.153
DDD	7698	20.694
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7698	324205	2.37

Instrument :
BNA_G
ClientSampleId :
DFTPP