
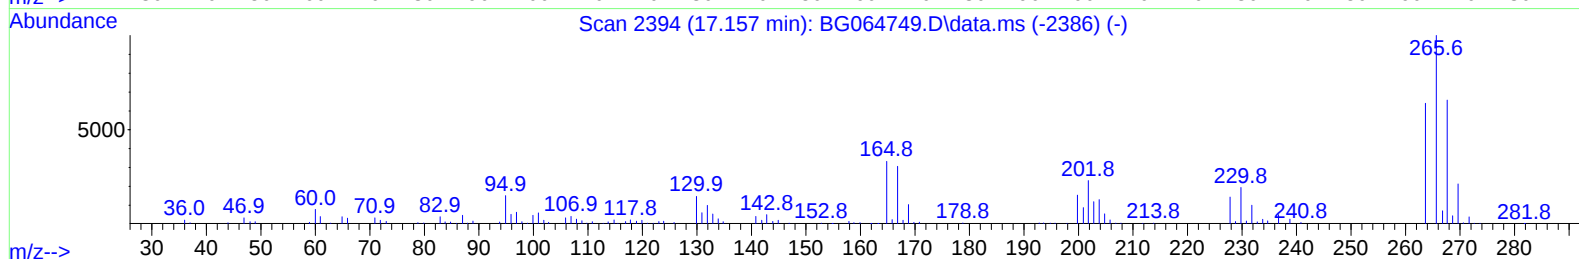
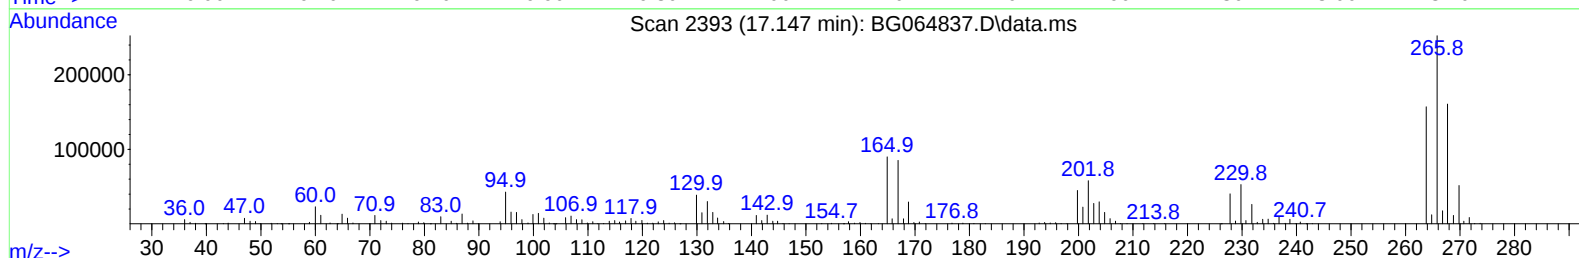


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064837.D
Acq On : 21 Nov 2025 9:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 10:03:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

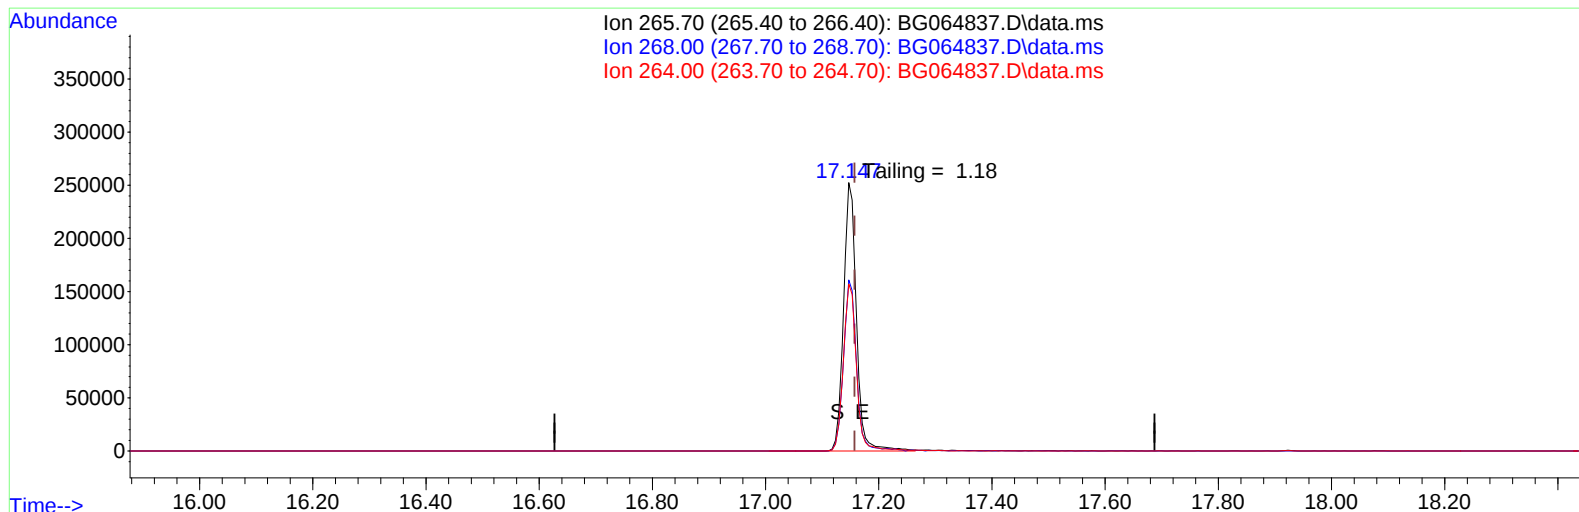

TIC: BG064837.D\data.ms

(70) Pentachlorophenol (C)




17.147min (-0.010) 696296.48 ng

response 397657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	63.73
264.00	64.00	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064837.D
Acq On : 21 Nov 2025 9:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 10:03:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

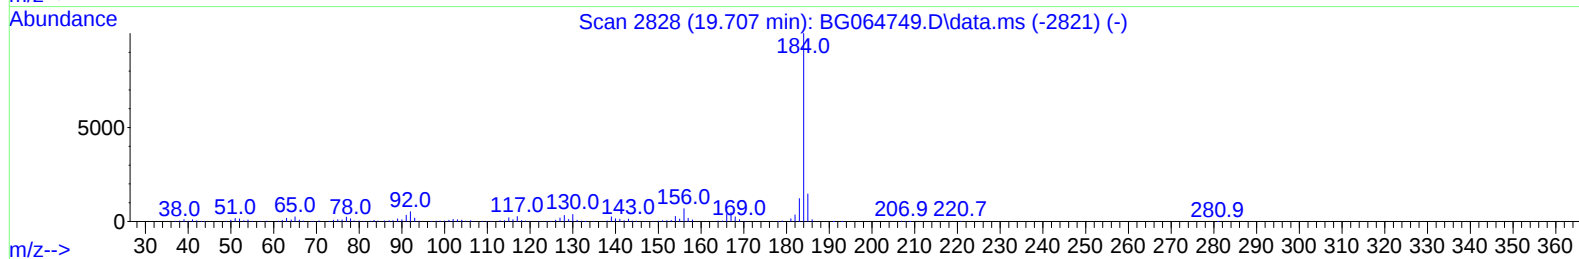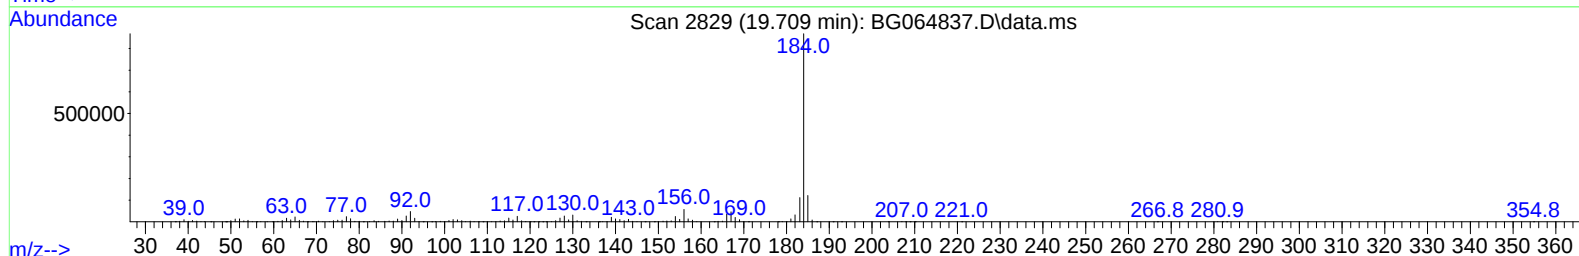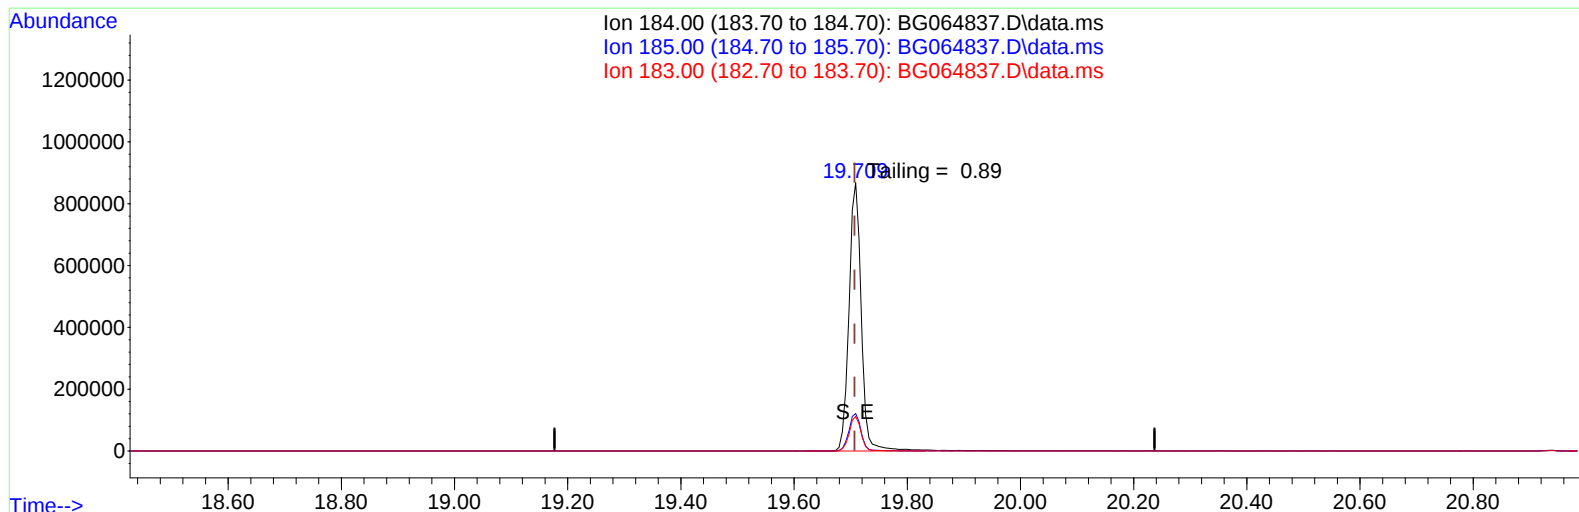

TIC: BG064837.D\data.ms

(77) Benzidine

19.709min (+ 0.002) 27434.59 ng

response 1309666

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.97
183.00	12.20	12.90
0.00	0.00	0.00